



## New biotite and muscovite isotopic reference materials, USGS57 and USGS58, for $\delta^2\text{H}$ measurements—A replacement for NBS 30



Haiping Qi<sup>a,\*</sup>, Tyler B. Coplen<sup>a</sup>, Matthias Gehre<sup>b</sup>, Torsten W. Vennemann<sup>c</sup>, Willi A. Brand<sup>d</sup>, Heike Geilmann<sup>d</sup>, Gerard Olack<sup>e</sup>, Ilya N. Bindeman<sup>f</sup>, Jim Palandri<sup>f</sup>, Li Huang<sup>g</sup>, Fred J. Longstaffe<sup>g</sup>

<sup>a</sup> U.S. Geological Survey, 431 National Center, Reston, VA 20192, USA

<sup>b</sup> Department for Isotope Biogeochemistry, Helmholtz-Centre for Environmental Research (UFZ), Permoserstrasse 15, 04318 Leipzig, Germany

<sup>c</sup> Institute of Earth Surface Dynamics, University of Lausanne, 1015, Switzerland

<sup>d</sup> Max-Planck-Institute for Biogeochemistry, Beutenberg Campus, P.O. Box 100164, 07701 Jena, Germany

<sup>e</sup> Department of the Geophysical Sciences, The University of Chicago, Chicago 60637, USA

<sup>f</sup> Department of Earth Sciences, University of Oregon, Eugene, OR 97403, USA

<sup>g</sup> Department of Earth Sciences, The University of Western Ontario, London, Ontario N6A 3K7, Canada

### ARTICLE INFO

#### Keywords:

HTC  
Hydrogen isotopes  
Isotope standards  
Hydrous minerals

### ABSTRACT

The advent of continuous-flow isotope-ratio mass spectrometry (CF-IRMS) coupled with a high temperature conversion (HTC) system enabled faster, more cost effective, and more precise  $\delta^2\text{H}$  analysis of hydrogen-bearing solids. Accurate hydrogen isotopic analysis by on-line or off-line techniques requires appropriate isotopic reference materials (RMs). A strategy of two-point calibrations spanning  $\delta^2\text{H}$  range of the unknowns using two RMs is recommended. Unfortunately, the supply of the previously widely used isotopic RM, NBS 30 biotite, is exhausted. In addition, recent measurements have shown that the determination of  $\delta^2\text{H}$  values of NBS 30 biotite on the VSMOW-SLAP isotope-delta scale by on-line HTC systems with CF-IRMS may be unreliable because hydrogen in this biotite may not be converted quantitatively to molecular hydrogen. The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of NBS 30 biotite analyzed by on-line HTC systems can be as much as 21 mUr (or ‰) too positive compared to the accepted value of  $-65.7$  mUr, determined by only a few conventional off-line measurements. To ensure accurate and traceable on-line hydrogen isotope-ratio determinations in mineral samples, we here propose two isotopically homogeneous, hydrous mineral RMs with well-characterized isotope-ratio values, which are urgently needed. The U.S. Geological Survey (USGS) has prepared two such RMs, USGS57 biotite and USGS58 muscovite. The  $\delta^2\text{H}$  values were determined by both glassy carbon-based on-line conversion and chromium-based on-line conversion, and results were confirmed by off-line conversion. The quantitative conversion of hydrogen from the two RMs using the on-line HTC method was carefully evaluated in this study. The isotopic compositions of these new RMs with 1- $\sigma$  uncertainties and mass fractions of hydrogen are:

USGS57 (biotite)

$\delta^2\text{H}_{\text{VSMOW-SLAP}} = -91.5 \pm 2.4$  mUr ( $n = 24$ )

Mass fraction hydrogen =  $0.416 \pm 0.002\%$  ( $n = 4$ )

Mass fraction water =  $3.74 \pm 0.02\%$  ( $n = 4$ )

USGS58 (muscovite)

$\delta^2\text{H}_{\text{VSMOW-SLAP}} = -28.4 \pm 1.6$  mUr ( $n = 24$ )

Mass fraction hydrogen =  $0.448 \pm 0.002\%$  ( $n = 4$ )

Mass fraction water =  $4.03 \pm 0.02\%$  ( $n = 4$ ).

These  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values encompass typical ranges for solid unknowns of crustal and mantle origin and are available to users for recommended two-point calibration.

### 1. Introduction

Hydrogen-isotope information obtained from hydrogen liberated

from hydroxyl-bearing minerals has been widely used to answer scientific questions on the petrogenesis of minerals and their host rocks (Suzuoki and Epstein, 1976), investigating topics in sedimentary

\* Corresponding author.

E-mail address: [haipingqi@usgs.gov](mailto:haipingqi@usgs.gov) (H. Qi).

geology and geochemistry (Savin and Epstein, 1970), tracking the origin of hydrous fluids at seismogenic depths (Mitterpergher et al., 2014) and water in volcanic glass (Seligman et al., 2016), evaluating fluid fluxes in silicic magmas (Deering et al., 2012), investigating ancient climate and hydrologic regimes (Abruzzese et al., 2005), or classifying CM and CR chondrites (Alexander et al., 2013). Before continuous-flow high temperature conversion (HTC) techniques (also called the on-line TC/EA method) were developed, off-line reduction of water with uranium or zinc metal to liberate molecular hydrogen by microwave (or other means of heating hydrogen-bearing silicates) served as the conventional method for hydrogen isotopic analysis of solids (Bigeleisen et al., 1952; Friedman, 1953; Godfrey, 1962; Coleman et al., 1982; Kendall and Coplen, 1985; Suzuoki and Epstein, 1976; Vennemann and O'Neil, 1993). Since the late 1990s, the advent of continuous-flow isotope-ratio mass spectrometry (CF-IRMS) coupled with a HTC system enabled faster, more cost effective, and sometimes also more precise  $\delta^2\text{H}$  analysis of hydrogen-bearing solids, gases, and water samples (Begley and Scrimgeour, 1996; Burgoyne and Hayes, 1998; Hilkert et al., 1999). This method benefits from the fact that only 1–20 mg of material is required, which is 50–200 mg less than that for the conventional off-line method, enabling (1) replication and triplication of measurements for improved precision, and (2) analysis of alteration-free specimens. Sharp et al. (2001) applied the CF-IRMS technique to hydrous minerals and developed a rapid method for  $\delta^2\text{H}$  measurements. Since then, many researchers have adapted and improved on-line HTC methods for hydrogen-isotope analysis of closed-system fluids, freshwater chert, silicic magmas, and various hydrous minerals (Marks et al., 2004; Abruzzese et al., 2005; Gong et al., 2007; Deering et al., 2012; Underwood et al., 2012; Bindeman et al., 2012; VanDeVelde and Bowen, 2013; Bauer and Vennemann, 2014; Mitterpergher et al., 2014; Seligman et al., 2016).

Stable hydrogen isotopic compositions are expressed as delta values denoted as  $\delta^2\text{H}_{\text{VSMOW}}$ , which is defined by the relation (Coplen, 2011):

$$\delta^2\text{H}_{\text{VSMOW}} = \frac{R(^2\text{H}/^1\text{H})_{\text{P}} - R(^2\text{H}/^1\text{H})_{\text{VSMOW}}}{R(^2\text{H}/^1\text{H})_{\text{VSMOW}}}$$

where  $R(^2\text{H}/^1\text{H})_{\text{P}}$  is the ratio  $N(^2\text{H})_{\text{P}} / N(^1\text{H})_{\text{P}}$  and  $N(^2\text{H})_{\text{P}}$  and  $N(^1\text{H})_{\text{P}}$  are the numbers of the two isotopes of hydrogen,  $^2\text{H}$  and  $^1\text{H}$ , respectively, in a sample P, and similarly for the reference VSMOW (Vienna Standard Mean Ocean Water). The International Union of Pure and Applied Chemistry (IUPAC) recommends that use of the per mil symbol (‰) be avoided (Cohen et al., 2007). Therefore, we follow the suggestion of Brand and Coplen (2012) and use the term urey (symbol Ur), which is suited for diverse isotope scales of all elements. One milliuery = 0.001 = 1‰. A delta value in the traditional form of  $-25\text{‰}$  can be expressed as  $-25 \text{ mUr}$ . The  $\delta^2\text{H}_{\text{VSMOW}}$  values herein are normalized on an isotope scale such that the  $\delta^2\text{H}$  value of SLAP (Standard Light Antarctic Precipitation) is  $-428 \text{ mUr}$  (Gonfiantini, 1978; Coplen, 1994), and they are identified as  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values.

Accurate hydrogen isotope analysis by on-line or off-line techniques requires appropriate isotopic reference materials (RMs). A strategy of two-point calibrations (Coplen, 1988; Coplen, 1994; Werner and Brand, 2001; Paul et al., 2007; Brand et al., 2014; Schimmelmann et al., 2009; Bindeman et al., 2012; Schimmelmann et al., 2016) using two RMs is recommended. However, only one internationally distributed mineral isotopic RM, NBS 30 biotite, exists. NBS 30 was prepared by I. Friedman, J. R. O'Neil, and G. Cebula (U.S. Geological Survey) from a sample of the Lakeview tonalite (Southern California batholith) provided by L. Silver (California Institute of Technology, Pasadena, California) (Gonfiantini, 1984), and its particle size ranges between 200 and 300  $\mu\text{m}$ . This material is intended for calibration of oxygen and hydrogen isotopic measurements of silicates and hydrous solids. The assigned  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  value of  $-65.7 \text{ mUr}$  for NBS 30 biotite is the average value obtained from measurements reported by Gonfiantini (1984) and Hut (1987). Prior to 2016, only a few other international

RMs existed for hydrogen isotopic analysis of solids, including IAEA-CH-7 polyethylene foil ( $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -99.2 \text{ mUr}$ ; Schimmelmann et al., 2016), NBS 22 oil ( $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -117.2 \text{ mUr}$ ; Schimmelmann et al., 2016), USGS42 Tibetan human hair ( $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -72.9 \text{ mUr}$ ; Coplen and Qi, 2016), and USGS43 Indian human hair ( $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -44.4 \text{ mUr}$ ; Coplen and Qi, 2016). The supplies of NBS 30 biotite and NBS 22 oil are exhausted, and polyethylene and human hair RMs are not suitable for  $\delta^2\text{H}$  measurements of hydrous minerals. Furthermore, determination of  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of NBS 30 biotite by established on-line HTC techniques was found to be unreliable because hydrogen conversion from this biotite proved to be non-quantitative (Qi et al., 2014a). The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of NBS 30 by three laboratories were as much as 21 mUr higher than the accepted value of  $-65.7 \text{ mUr}$ , determined by conventional off-line measurements. Further experiments revealed a strong correlation between grain size and  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  of NBS 30 biotite, but not of biotites with lower iron content. Moreover, the  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of NBS 30 as a function of particle size showed a clear trend toward  $-65.7 \text{ mUr}$  with finer grain size (Qi et al., 2014a). In 2016, 19 new organic RMs for hydrogen, carbon, and nitrogen stable isotope-ratio measurements were prepared (Schimmelmann et al., 2016), and these enabled more accurate determinations of relative stable isotope ratios of hydrogen ( $\delta^2\text{H}$ ), carbon ( $\delta^{13}\text{C}$ ), and nitrogen ( $\delta^{15}\text{N}$ ) measurements using at least two isotopic RMs to anchor the isotope-delta scale with RMs having strongly contrasting isotopic compositions (Coplen, 1988; Coplen, 1996; Paul et al., 2007; Brand et al., 2014). However, none of the 19 RMs is suitable for hydrogen isotopic analysis of minerals because of differences in the material matrix.

Although a conventional on-line HTC method using a glassy carbon-filled reactor (C-EA) has enabled faster, more cost-effective measurements of hydrogen and oxygen isotopes in a wide range of solid materials, accurate  $\delta^2\text{H}$  measurements of many materials have been found to be problematic (Armbruster et al., 2006; Hunsinger et al., 2013; Qi et al., 2014a; Gehre et al., 2015; Nair et al., 2015; Gehre et al., 2017). Besides the problem exemplified by NBS 30 biotite mentioned above, the formation of hydrogen-bearing by-products, such as HCN and HCl (HX), was verified when nitrogen-, chlorine-, and sulfur-bearing organic materials were analyzed by conventional on-line HTC (Hunsinger et al., 2013; Gehre et al., 2015; Nair et al., 2015; Gehre et al., 2017). The formation of hydrogen-bearing by-products prevents a quantitative conversion of organically bound hydrogen in samples to the analyte  $\text{H}_2$ . Thus,  $\delta^2\text{H}$  results are seriously compromised because of isotopic fractionation. To overcome this problem, Gehre et al. (2015) have modified the conventional on-line HTC method that uses a glassy, carbon-filled reactor. They developed a method employing a chromium-filled, high-temperature reactor (Cr-EA). This method minimizes the production of intermediately formed hydrogen-bearing by-products (HCN, HCl) enabling quantitative conversion to molecular hydrogen. Gehre et al. (2017) later improved the Cr-EA method and extended the investigation of  $\delta^2\text{H}$  analysis to substances containing fluorine, chlorine, bromine, iodine, and sulfur. The optimized the EA-Cr/HTC-IRMS technique, which offers more accurate  $\delta^2\text{H}$  analysis of fluorine-, chlorine-, bromine-, iodine-, and sulfur-bearing substances.

To ensure accurate and traceable on-line  $\delta^2\text{H}$  determination of mineral samples, two isotopically homogeneous hydrous mineral RMs with well-characterized  $\delta^2\text{H}$  values are needed. The USGS has prepared two such RMs, USGS57 biotite and USGS58 muscovite, both from China. At the same time, the quantitative conversion of hydrogen from these two RMs was carefully evaluated using on-line C-EA and Cr-EA methods, as well as off-line conversion (Kokubu et al., 1961). Seven laboratories participated in this study. Sample preparation methods and methods to determine  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values are described in this article.

## 2. Selection of two mineral isotopic reference materials

Two phyllosilicate RMs having  $\delta^2\text{H}$  values sufficiently different to encompass most natural hydrous minerals were sought. Five powdered biotites and four muscovites with different particle sizes ranging from 74 to 250  $\mu\text{m}$  (200 to 60 mesh) were purchased from Antai Mining Co., Ltd. (Lingshou County, Shijiazhuang, Hebei Province, China). The biotite and muscovite were separated from natural rocks in China and crushed in an industrial-scale factory. The biotite with particle size of 177  $\mu\text{m}$  (80 mesh) and the muscovite with particle size of 149  $\mu\text{m}$  (100 mesh) were found to be suitable RMs, and they were designated as USGS57 and USGS58, respectively. About 2 kg of each material was tumbled in a large glass jar for seven days to ensure isotopic homogeneity of the different mineral grains.

## 3. Experimental methods

### 3.1. The isotopic reference materials

The isotopic RMs VSMOW, VSMOW2, SLAP2, GISP, NBS 22 oil ( $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -117.2$  mUr; Schimmelmann et al., 2016), and USGS47 ( $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -150.2$  mUr; Qi et al., 2014b) were sealed in silver tubes using a semi-automated sealing technique (Qi et al., 2010). The selected reference samples were distributed to the other participating laboratories. All laboratories used combinations of primary and secondary international measurement standards for two-point calibrations. Each laboratory also analyzed their in-house RMs to ensure the quality of  $\delta^2\text{H}$  measurements. USGS62 caffeine ( $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -156.1$  mUr; Schimmelmann et al., 2016) and USGS77 polyethylene powder ( $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -75.9$  mUr; Schimmelmann et al., 2016) were used to quantify the mass fraction of hydrogen by a Cr-filled reactor.

### 3.2. The $\delta^2\text{H}_{\text{VSMOW-SLAP}}$ determination

Six of the laboratories used a variety of analytical approaches for  $\delta^2\text{H}$  measurements using on-line conversion with EA-C/HTC or EA-Cr/HTC methods, and one laboratory performed  $\delta^2\text{H}$  analysis with an off-line method.

At the Reston Stable Isotope Laboratory (RSIL), the  $\delta^2\text{H}$  measurements were made with a HTC (TC/EA, Thermo-Finnigan, Bremen, Germany) reduction unit equipped with a Costech Zero-Blank 100-position Autosampler (Costech, Valencia, California), a ConFlo IV gas introduction system (Thermo Fisher, Bremen, Germany), and a Delta<sup>plus</sup> XP isotope-ratio mass spectrometer (Thermo, Bremen, Germany). The details of the method using a glassy carbon-filled reactor were described by Qi et al. (2014a). For early measurements with a Cr-filled reactor, the method described in Method #2 of Table 1 was used. Subsequently, for samples analyzed with a Cr-filled reactor, the glassy carbon tube inside the ceramic tube that is normally filled with glassy carbon chips was packed with a mixture of chromium and glassy carbon chips. The mix ratio of chromium chips to glassy carbon chips was about 1:1 by volume. The bottom 35 mm of the ceramic tube was filled with chromium and glassy carbon chips and was supported by silver wool. The helium carrier gas (100 mL min<sup>-1</sup>) was fed from the top, as originally supplied. The reactor temperature was set to values between 1050 to 1450 °C, and the GC temperature was maintained at 80 °C.

Solid mineral samples were weighed into silver capsules. Reference waters and oil contained the same amount of hydrogen as found in mineral samples, and these liquids were crimp-sealed into segments of silver tubes, interspersed with unknown samples, and analyzed as solid samples (Qi et al., 2010). The use of reference waters in silver tubes made it possible to measure  $\delta^2\text{H}$  values of mineral materials directly against reference waters with known  $\delta^2\text{H}$  values (Coplen and Qi, 2010) following the principle of identical treatment (Werner and Brand, 2001).

For the other laboratories, the on-line methodologies were based on a variety of high temperature conversion elemental analyzer (HTC) and gas chromatographic (GC) interfaces, as well as mass spectrometers from different manufacturers; see the summary in Table 1.

For off-line analysis, structural hydrogen was extracted from RMs using a method modified after Godfrey (1962), Kyser and O'Neil (1984), and Vennemann and O'Neil (1993). Briefly, ~70 mg of muscovite or biotite were loaded into a quartz tube and outgassed for 12 h at 200 °C to remove adsorbed water. The sample was then heated using a fuel-gas-oxygen torch for ~10 min during which released H<sub>2</sub>O was trapped at -196 °C. Gas initially released as H<sub>2</sub> was oxidized over copper oxide (CuO) at 550 °C to form H<sub>2</sub>O, which was also collected in the -196 °C trap. The total water collected was then reacted with powdered chromium at 900 °C to produce H<sub>2</sub>, which was collected on charcoal at -196 °C and the yield of H<sub>2</sub> was measured. The H<sub>2</sub> was analyzed using a Thermo Scientific Delta<sup>plus</sup> XL dual-inlet IRMS. Values of  $\delta^2\text{H}$  were calibrated to the VSMOW-SLAP scale using 3-mL volumes of VSMOW and USGS47. The water standards were treated in an identical fashion to the total water released from the RMs.

## 4. Results and discussion

### 4.1. Isotopic homogeneity and evaluation of chemical purity of the two RMs

The evaluation for isotopic homogeneity was only performed by the RSIL. Fifteen vials of each RM were selected randomly, labeled as vial #1 through vial #15. The  $\delta^2\text{H}$  values of three aliquots from each vial of USGS57 and USGS58 were determined (Table 2). Two different sample amounts were analyzed in the Cr-filled reactor and the glassy carbon-filled reactor (Table 2). The sample masses for the Cr-filled reactors contained ~1.8 mg (equivalent to 0.07  $\mu\text{L}$  of water or 7.8  $\mu\text{g}$  of hydrogen). The sample masses of USGS57 and USGS58 for the glassy carbon-filled reactor were 3.56 and 3.25 mg, respectively (both equivalent to 0.15  $\mu\text{L}$  of water or 16.7  $\mu\text{g}$  of hydrogen). To account for  $\delta^2\text{H}$  drift resulting from residue buildup over time, each analysis run was controlled by analyzing two or more aliquots of the RM from vial #1 at the beginning, the middle, and the end of the run. No drift in  $\delta^2\text{H}$  values was observed from any of the four runs. The standard deviations of the larger-sample masses (for the glassy carbon-filled reactor) were better than those of the smaller-sample masses (for the Cr-filled reactor). For example, the mean values of the 15 standard deviations of USGS57 and USGS58 analyzed using the glassy carbon-filled reactor were 0.7 and 0.5 mUr, respectively. The mean values of the 15 standard deviations of USGS57 and USGS58 analyzed using the Cr-filled reactor were 1.4 and 1.3 mUr, respectively. There are a few vials that appeared to have higher standard deviations for  $\delta^2\text{H}$  values in Table 2, for example, between 2.6 and 3.4 mUr when small amounts of material were analyzed. It is not clear whether this higher standard deviation only reflects material homogeneity inside the respective vial or whether it was the result of the analytical measurement with a smaller amount of sample. Because these two mineral materials were produced in an industry-scale factory, we cannot rule out that small particles with substantially different  $\delta^2\text{H}$  values may be mixed in the RMs. To be cautious, it is recommended that at least two or three of the same RM be analyzed at the beginning, the middle, and the end of a run with an amount of hydrogen no < 16.7  $\mu\text{g}$ . Nevertheless, the average standard deviations of the averages of the 15 measurements of USGS57 and USGS58 shown in Table 2 are 1.1 and 0.6 mUr, respectively, demonstrating that the two RMs are isotopically homogeneous for amounts of material as small as 3.56 and 3.25 mg, respectively.

The mineralogical purity of USGS57 and USGS58 was evaluated by X-ray diffraction at the USGS, Reston. USGS57 contains 98% biotite by mass and USGS58 contains 97% muscovite by mass (Table 3).

**Table 1**  
Stable isotope analytical methods and equipment of participating laboratories.

Laboratory	Instruments	Method and condition
University of Chicago, Chicago, USA	On-line, Thermo Scientific Delta V PLUS IRMS, Thermo Scientific HTC connected via Thermo ConFlo IV interface	Glassy carbon tube filled with glassy carbon chips without graphite crucible. Reactor 1450 °C, GC 90 °C, helium flow 100 mL min <sup>-1</sup>
Stable Isotope Laboratory, University of Lausanne, Switzerland	On-line, Thermo Scientific Delta <sup>plus</sup> XL IRMS, Thermo Scientific HTC connected via Thermo ConFlo III interface	Glassy carbon tube filled with glassy carbon chips with graphite crucible. Reactor 1450 °C, GC 85 °C, helium flow ~90 mL min <sup>-1</sup>
University of Oregon, Eugene, Oregon, USA	Online Thermo Scientific MAT253 IRMS and HTC system	Glassy carbon chips and oven, 1450 °C, GC at 70 °C during run, 300 °C overnight prior to analytical session. Helium flow 80 mL min <sup>-1</sup> (Martin et al., 2017)
UFZ, Helmholtz-Centre for Environmental Research, Leipzig, Germany	On-line Euro 3000 Elemental Analyzer (Eurovector, Italy), Connected via Thermo ConFlo IV to a Thermo Scientific MAT 253 <sup>TM</sup> IRMS	Quartz oven filled with chromium, one-oven system, 1150–1270 °C, helium flow ~100 mL min <sup>-1</sup> (Gehre et al., 2015)
MPI-BGC, Max Planck Institute for Biogeochemistry, Jena, Germany	On-line, Hekatech HTC connected via Thermo ConFlo III interface to Thermo Scientific Delta <sup>plus</sup> XL IRMS	Oven filled with a mixture of chromium and glassy carbon chips, one-oven system, 1400–1450 °C, helium carrier gas ~80 mL min <sup>-1</sup> with reversed flow (Gehre et al., 2004, Nair et al., 2015)
RSIL, U.S Geological Survey, Reston, Virginia, USA	On-line, Thermo Scientific Delta <sup>plus</sup> XP IRMS, Thermo Scientific HTC connected via Thermo ConFlo IV interface	Method #1: Glassy carbon tube filled with glassy carbon chips without graphite crucible. Reactor 1450 °C, GC 80 °C, helium flow 120 mL min <sup>-1</sup> . Method #2: Removed glassy carbon tube. Filled ceramic tube from bottom to top with glassy carbon chips, quartz wool and 3 cm of chromium powder. Reactor 1150 °C, GC 80 °C, helium flow 120 mL min <sup>-1</sup>
Laboratory for Stable Isotope Science, The University of Western Ontario, London, Ontario, Canada	Manual dual-inlet measurements using a Thermo Scientific Delta <sup>plus</sup> XL dual-inlet IRMS	Off-line heating in evacuated quartz tubes using a fuel-gas oxygen torch (Vennemann and O'Neil, 1993); released water trapped at -196 °C, and released H <sub>2</sub> oxidized over CuO at 550 °C and combined with released water; reduction of H <sub>2</sub> O to H <sub>2</sub> with chromium at 900 °C; collection of analyte H <sub>2</sub> on charcoal at -196 °C and measurement of yield (Godfrey, 1962; Kyser and O'Neil, 1984). All performed using a vacuum line.

#### 4.2. Particle size, chromium- and glassy carbon-filled reactors, and drying test

Work by Qi et al. (2014a) demonstrated that determination of  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of NBS 30 biotite with on-line HTC systems with glassy carbon-filled reactors was unreliable because hydrogen conversion from this specific biotite RM was not quantitative. Experiments have shown that the  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of NBS 30 demonstrate a clear trend toward -65.7 mUr with finer grain size. The difference in  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values obtained from NBS 30 with original particle size and that with a finer particle size can be as high as 21 mUr (Qi et al.,

2014a). In addition, Hunsinger et al. (2013), Gehre et al. (2015) and Nair et al. (2015) established that hydrogen isotopic results can be seriously compromised when N-, Cl-, S-bearing organic materials are analyzed by a conventional on-line HTC method (with a glassy carbon-filled reactor) because of isotopic fractionation caused by the formation of hydrogen-bearing by-products, such as HCN and HCl. To overcome this problem, Gehre et al. (2015) modified the conventional glassy-carbon on-line HTC method by using elemental chromium (Cr-EA). This method prevents hydrogen-bearing by-products (HCN and HCl) from surviving in the reactor and enables quantitative conversion of hydrogen from organic matter to molecular hydrogen. Gehre et al. (2017)

**Table 2**  
Hydrogen isotopic homogeneity of USGS57 biotite and USGS58 muscovite.  
[The  $\delta^2\text{H}$  values are measured, not scale-normalized values.]

Sample	USGS57 biotite		USGS58 muscovite	
	Cr-packed reactor <sup>a</sup>	Glassy carbon-packed reactor <sup>b</sup>	Cr-packed reactor <sup>a</sup>	Glassy carbon-packed reactor <sup>b</sup>
	$\delta^2\text{H}$ (mUr)	$\delta^2\text{H}$ (mUr)	$\delta^2\text{H}$ (mUr)	$\delta^2\text{H}$ (mUr)
#1	-90.1 ± 1.3	-94.3 ± 0.8	-28.4 ± 1.4	-29.5 ± 0.3
#2	-90.0 ± 1.3	-94.3 ± 1.4	-29.2 ± 0.4	-29.6 ± 0.7
#3	-89.2 ± 0.7	-94.3 ± 0.7	-27.9 ± 1.3	-29.6 ± 0.6
#4	-90.8 ± 0.9	-93.8 ± 0.3	-28.0 ± 1.4	-29.7 ± 0.7
#5	-91.1 ± 1.1	-94.3 ± 0.2	-27.9 ± 0.6	-30.2 ± 0.7
#6	-89.9 ± 2.6	-93.8 ± 0.2	-28.2 ± 0.9	-29.8 ± 0.4
#7	-91.1 ± 1.3	-94.3 ± 0.2	-27.1 ± 3.4	-30.0 ± 0.3
#8	-91.5 ± 0.4	-94.3 ± 0.6	-28.0 ± 1.1	-30.1 ± 0.3
#9	-90.1 ± 3.3	-93.9 ± 0.9	-28.8 ± 0.3	-29.7 ± 0.6
#10	-90.2 ± 0.8	-94.8 ± 1.0	-27.0 ± 0.5	-29.4 ± 0.8
#11	-91.0 ± 1.9	-94.1 ± 0.5	-27.0 ± 3.1	-28.8 ± 0.5
#12	-91.4 ± 2.0	-94.0 ± 0.8	-28.4 ± 1.1	-30.1 ± 0.7
#13	-92.9 ± 0.4	-92.1 ± 2.6	-28.2 ± 1.9	-29.3 ± 0.5
#14	-92.0 ± 1.3	-89.7 ± 0.5	-28.2 ± 1.1	-29.3 ± 0.4
#15	-92.3 ± 0.9	-93.0 ± 0.5	-27.1 ± 0.2	-28.9 ± 0.3
average	-91.0 ± 0.9	-93.8 ± 1.2	-28.0 ± 0.7	-29.6 ± 0.4

<sup>a</sup> The amount of material used for these analyses contain hydrogen equivalent to hydrogen in 0.07  $\mu\text{L}$  of water.

<sup>b</sup> The amount of material used for these analyses contains hydrogen extracted from the equivalent of 0.15  $\mu\text{L}$  of water.



**Table 3**

The mass fractions of biotite, muscovite, and other minerals in USGS57 and USGS58.

[Ideal formulae: biotite,  $K(Mg,Fe)_3AlSi_3O_{10}(OH)_2$ ; muscovite,  $KAl_2(AlSi_3O_{10})(OH)_2$ ; K-feldspar,  $KAlSi_3O_8$ ; quartz,  $SiO_2$ ; plagioclase, solid solution of  $NaAlSi_3O_8$  and  $CaAl_2Si_2O_8$ ; chlorite,  $Mg_3(Si_4O_{10})(OH)_2 \cdot Mg_3(OH)_6$ .]

Name	Material	Mass fraction					
		Biotite	Muscovite	K-feldspar	Quartz	Plagioclase	Chlorite
USGS57	Biotite 80 mesh	0.98		Trace	Trace	0.01	0.01
USGS58	Muscovite 100 mesh		0.97	0.01	Trace	0.02	Trace

further improved the Cr-EA method and extended the investigation of hydrogen isotopic analysis to substances containing fluorine, chlorine, bromine, iodine, and sulfur. The optimized EA-Cr/HTC-IRMS technique offers more accurate hydrogen isotopic analysis of fluorine-, chlorine-, bromine-, iodine-, and sulfur-bearing substances.

To evaluate the effect of variation in particle size of RMs using the on-line HTC systems, different size fractions of the two new RMs were analyzed with both the Cr-filled and glassy carbon-filled reactors. Samples of USGS57 biotite and USGS58 muscovite (original particle sizes of 177  $\mu$ m and 149  $\mu$ m, respectively) were ground, and different size fractions were collected. Four aliquots from each size fraction of each material were weighed as the first set for our evaluation. Another set of samples identical to the first set was also weighed. Half of samples from each size fraction from the second set were dried in a vacuum oven at 70 °C overnight, and half remained undried. The first set of samples was analyzed by a conventional HTC with the glassy carbon-filled reactor method (Qi et al., 2014a). The second set with dried and undried samples was analyzed by an HTC with the Cr-filled reactor. The measured  $\delta^2H$  values (not scale-normalized values) and relative peak area to mass values (relative total  $H_2$  peak areas divided by the theoretical mass of hydrogen in the analyzed material) from the different particle size fractions are summarized in Table 4. There are no measurable differences in  $\delta^2H$  values or in relative hydrogen yields (relative peak area to mass) between dried and undried USGS57 and USGS58 for the same particle size (Table 4), as determined with the Cr-filled reactor. This demonstrates that USGS57 biotite and USGS58 muscovite do not absorb detectable amounts of moisture under normal laboratory conditions. However, measured  $\delta^2H$  values and relative hydrogen yields vary with particle size for both USGS57 biotite (Fig. 1a) and USGS58 muscovite (Fig. 1b). This indicates that the two materials behaved differently in the HTC system, presumably because of the different

chemical compositions of USGS57 and USGS58. For USGS57 biotite, the amount of hydrogen released from the same amount of material increased and the  $\delta^2H$  value decreased with finer particle size in the range of 74–177  $\mu$ m (Fig. 1a). This pattern is similar to the pattern shown by NBS 30 biotite (Qi et al., 2014a). Interestingly, when the particle size of USGS57 was smaller than 74  $\mu$ m, the relative hydrogen yield decreased from the highest value of 17.91 to 17.08 and the lowest  $\delta^2H$  value of  $-98.4$  mUr was obtained. For USGS58 muscovite, the highest relative hydrogen yield and most positive  $\delta^2H$  values were measured for the particle size between 105–149  $\mu$ m (Fig. 1b). Like USGS57, when particle size of USGS58 was smaller than 74  $\mu$ m, the relative hydrogen yield also decreased from the highest value of 20.51 (dried) and 20.37 (undried) to 18.64 (dried) and 18.62 (undried), respectively, and the lowest  $\delta^2H$  values of  $-34.4$  mUr (dried) and  $-33.4$  mUr (undried) were obtained. When undried samples from different particle sizes were analyzed using the glassy carbon-filled reactor, the patterns of  $\delta^2H$  values and relative hydrogen yields are very similar to those determined with the Cr-filled reactor for both USGS57 (Fig. 1c) and USGS58 (Fig. 1d). The  $\delta^2H$  values of USGS57 biotite analyzed with the glassy carbon-filled reactor may be more consistent with an average value of  $-94.3 \pm 0.3$  mUr compared to the value of  $-96.5 \pm 1.2$  mUr (dried) or  $-97.2 \pm 1.1$  mUr (undried) for the Cr-filled reactors. The variation of the relative hydrogen yields with particle size was similar for both types of reactors (Table 4).

#### 4.3. Determination of mass fraction of hydrogen

Two independent analysis runs with different reactor filling (Cr-filled or glassy carbon-filled) were carried out to quantify the mass fractions of hydrogen in the two RMs. By comparing the mass fraction of hydrogen in dried and undried USGS57 and USGS58 with the

**Table 4**

Variation in measured  $\delta^2H$  values and relative hydrogen yields (relative peak area / mass) of USGS57 biotite and USGS58 muscovite having different particle sizes and drying conditions. [Standard deviations are one sigma;  $\delta^2H$  values are measured, not scale normalized.]

Method	Treatment	Particle size ( $\mu$ m)	USGS57 biotite		USGS58 muscovite		
			$\delta^2H$ (mUr)	Relative hydrogen yield	$\delta^2H$ (mUr)	Relative hydrogen yield	
Cr	Dried	Original	$-95.5 \pm 0.2$	$17.47 \pm 0.12$	$-31.8 \pm 0.9$	$19.72 \pm 0.05$	
		> 149	$-95.6 \pm 1.3$	$17.70 \pm 0.19$	$-28.3 \pm 0.3$	$20.34 \pm 0.05$	
	Dried	105–149	$-96.2 \pm 1.4$	$17.84 \pm 0.02$	$-27.6 \pm 1.3$	$20.51 \pm 0.34$	
		74–105	$-96.9 \pm 1.3$	$17.91 \pm 0.02$	$-30.3 \pm 0.0$	$19.74 \pm 0.02$	
	Dried	< 74	$-98.4 \pm 0.6$	$17.08 \pm 0.00$	$-34.4 \pm 0.2$	$18.64 \pm 0.05$	
		Average	$-96.5 \pm 1.2$	$17.60 \pm 0.34$	$-30.5 \pm 2.7$	$19.79 \pm 0.73$	
	Undried	Original	$-96.4 \pm 0.3$	$17.41 \pm 0.01$	$-30.6 \pm 1.4$	$19.54 \pm 0.09$	
		> 149	$-96.2 \pm 0.3$	$17.73 \pm 0.08$	$-28.7 \pm 0.3$	$20.37 \pm 0.08$	
	Undried	105–149	$-97.3 \pm 0.2$	$17.83 \pm 0.13$	$-27.9 \pm 0.1$	$20.25 \pm 0.09$	
		74–105	$-97.3 \pm 1.6$	$17.99 \pm 0.01$	$-28.8 \pm 1.1$	$19.81 \pm 0.07$	
	Undried	< 74	$-99.0 \pm 0.5$	$17.11 \pm 0.05$	$-33.4 \pm 0.9$	$18.62 \pm 0.09$	
		Average	$-97.2 \pm 1.1$	$17.62 \pm 0.36$	$-29.9 \pm 2.2$	$19.72 \pm 0.70$	
	Glassy carbon	Undried	Original	$-93.9 \pm 1.0$	$16.01 \pm 0.17$	$-31.2 \pm 1.1$	$18.05 \pm 0.12$
			> 149	$-94.3 \pm 0.3$	$16.22 \pm 0.06$	$-28.1 \pm 0.4$	$18.94 \pm 0.04$
Undried		105–149	$-94.5 \pm 0.3$	$16.43 \pm 0.09$	$-28.0 \pm 0.4$	$18.79 \pm 0.07$	
		74–105	$-94.2 \pm 0.5$	$16.51 \pm 0.10$	$-28.8 \pm 1.2$	$18.43 \pm 0.11$	
Undried		< 74	$-94.6 \pm 0.5$	$15.67 \pm 0.08$	$-32.1 \pm 0.3$	$17.46 \pm 0.11$	
		Average	$-94.3 \pm 0.3$	$16.17 \pm 0.34$	$-29.6 \pm 1.9$	$18.33 \pm 0.60$	

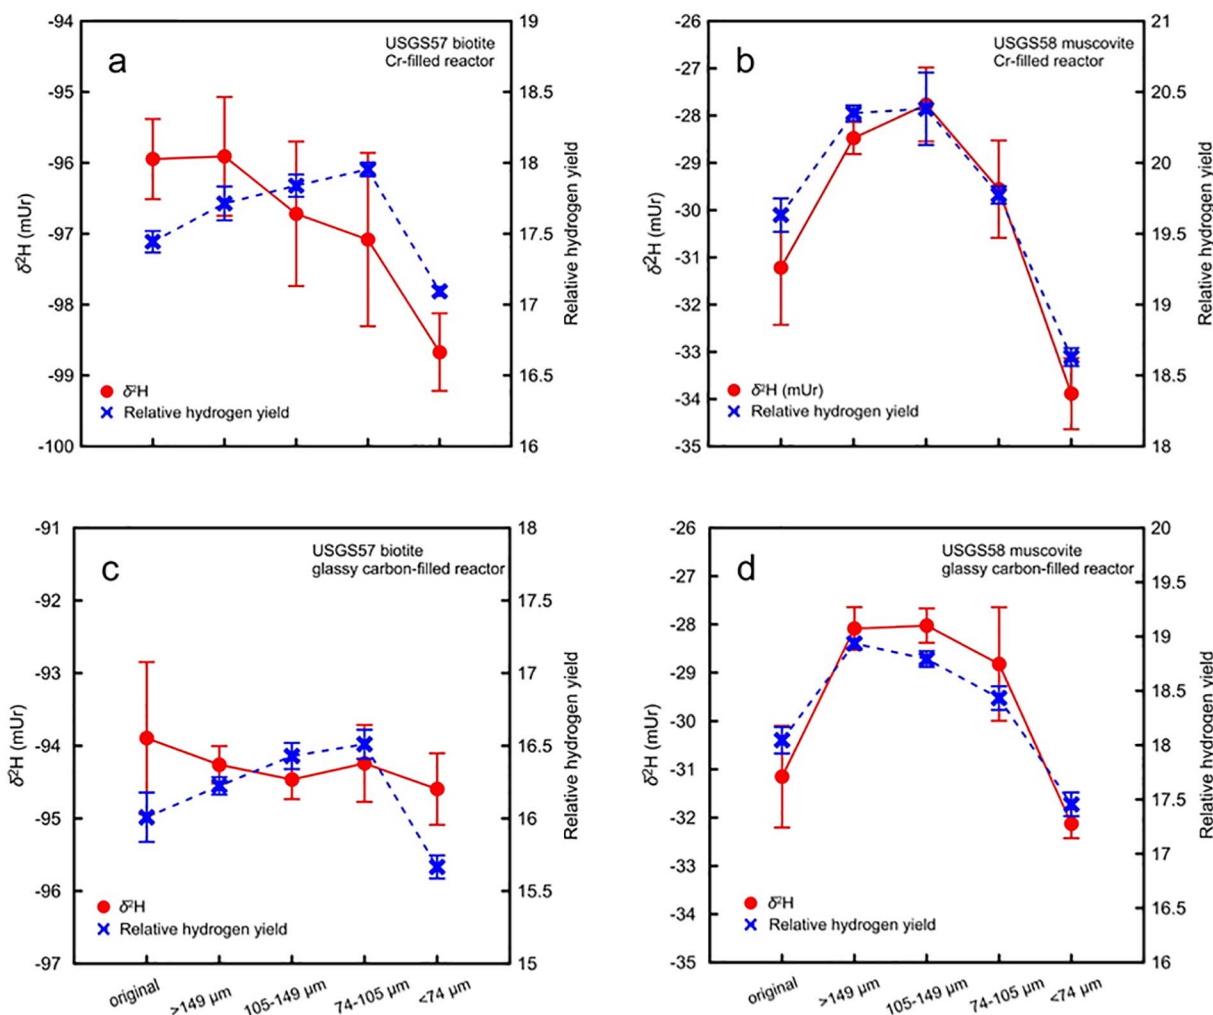


Fig. 1. Variation in  $\delta^2\text{H}$  value and relative hydrogen yield with a Cr-filled reactor of USGS57 biotite (a) and USGS58 muscovite (b) as a function of particle size; variation in  $\delta^2\text{H}$  value and relative hydrogen yield with a glassy carbon-filled reactor of USGS57 biotite (c) and USGS58 muscovite (d) as a function of particle size. Each data point is an average value of four analyses. The data in figure (a) and figure (b) are the combined results for analyses obtained in two dried samples and two undried samples. The  $\delta^2\text{H}$  values are measured, not scale normalized values.

Table 5

Hydrogen mass fractions of USGS57, USGS58, and NBS 30 as a function of particle size and drying conditions.

[Measurements determined with both a Cr-filled reactor (except NBS 30 was not included) and a glassy carbon-filled reactor; uncertainties are 1-sigma standard deviations.]

Reactor	Particle size ( $\mu\text{m}$ )	USGS57 biotite				USGS58 muscovite				NBS 30 biotite	
		Dried		Undried		Dried		Undried		Dried	
		As H (%)	As H <sub>2</sub> O (%)	As H (%)	As H <sub>2</sub> O (%)	As H (%)	As H <sub>2</sub> O (%)	As H (%)	As H <sub>2</sub> O (%)	As H (%)	As H <sub>2</sub> O (%)
Cr-filled <sup>a</sup>	Original	0.425	3.82	0.423	3.81	0.479	4.31	0.475	4.27	–	–
	149–177 or 149	0.430	3.87	0.431	3.88	0.494	4.44	0.494	4.45	–	–
	105–149	0.434	3.90	0.433	3.90	0.498	4.48	0.491	4.42	–	–
	74–105	0.435	3.92	0.437	3.93	0.479	4.31	0.481	4.33	–	–
	< 74	0.416	3.74	0.416	3.75	0.454	4.08	0.453	4.08	–	–
Glassy carbon-filled <sup>b</sup>	Original	0.416	3.74	–	–	0.432	3.89	–	–	0.395	3.55
	< 74	0.409	3.68	–	–	0.448	4.03	–	–	0.475	4.27
Recommended mass fraction H <sup>c</sup>		0.416 $\pm$ 0.002%, n = 4				0.448 $\pm$ 0.002%, n = 4				0.475 $\pm$ 0.015%, n = 4	
Recommended mass fraction H <sub>2</sub> O		3.74 $\pm$ 0.02%, n = 4				4.03 $\pm$ 0.02%, n = 4				4.27 $\pm$ 0.14%, n = 4	

<sup>a</sup> Measurements determined with a Cr-filled reactor; calculations were based on the yield of hydrogen from caffeine.

<sup>b</sup> Measurements determined with a glassy carbon-filled reactor; calculations were based on the yield of hydrogen from polyethylene.

<sup>c</sup> The recommended mass fractions of hydrogen (H) and water (H<sub>2</sub>O) were based on the assumption that the highest yield should provide most accurate values.

analytical run that used the Cr-filled reactor, we evaluated (1) the molecular hydrogen yields from different particle-size fractions of each material, and (2) the potential fraction of absorbed water. Several aliquots of caffeine having precisely determined masses were analyzed to

quantify the mass of hydrogen in the RMs. USGS62 caffeine samples were also analyzed at the beginning, the middle, and the end of a run to account for drift in the measurement of hydrogen yield. Samples of USGS57 biotite (original size 177  $\mu\text{m}$ ) and USGS58 muscovite (original

size 147  $\mu\text{m}$ ) were ground, and size fractions, ranging from 177  $\mu\text{m}$  to  $\leq 74 \mu\text{m}$ , were collected and analyzed. Two sets of samples with two aliquots of each size fraction of each RM were prepared. One set of samples was dried in a vacuum oven at 70 °C overnight with caffeine samples. The two sets of samples were analyzed in the same run with a Cr-filled reactor. The results (Table 5) indicate that there is no difference in the mass fraction of hydrogen determined with dried or with undried samples of USGS57 and USGS58. These results demonstrate that USGS57 biotite and USGS58 muscovite do not absorb detectable amount of moisture under normal laboratory conditions. However, the hydrogen yield varied with different particle-size fractions. For USGS57 biotite, with the results from both dried and undried samples, the hydrogen yield increased from 0.42% (3.82% as  $\text{H}_2\text{O}$ ) to 0.44% (3.92% as  $\text{H}_2\text{O}$ ) as the particle fraction decreased from the original size of 177  $\mu\text{m}$  to 74  $\mu\text{m}$ . From both dried and undried samples of USGS58 muscovite, the highest hydrogen yield was obtained from samples with particle-size fraction between 105  $\mu\text{m}$  and 149  $\mu\text{m}$ . It is interesting that hydrogen yield (as hydrogen) substantially decreased for particle-size fractions smaller than 74  $\mu\text{m}$  for both USGS57 and USGS58. The reason is unclear. We speculate that a chemical reaction occurred when very fine mineral powders were in contact with the chromium or glassy carbon reactor. Alternatively, it is possible that hydrogen in the fine-grained minerals, exposed at high temperature ( $> 1250 \text{ }^\circ\text{C}$ ) under reducing conditions is not released as molecular hydrogen because a small fraction of this hydrogen is strongly bonded to other elements in the mineral. In a second run in which a glassy carbon-filled reactor was used, we only analyzed original materials and the fraction with particle size smaller than 74  $\mu\text{m}$  of USGS57, USGS58, and NBS 30 of dried materials. In this run, several aliquots of polyethylene powder, USGS77 having precisely determined masses, were analyzed to quantify the mass of hydrogen in the RMs. The calculated values of the mass fraction of hydrogen were lower than the values obtained in the Cr-filled reactor run calculated by caffeine for both USGS57 and USGS58 (Table 5). We suspect that quantitative conversion of hydrogen from caffeine in the Cr-filled reactor was not complete. Thus, higher mass fraction values of hydrogen in USGS57 and USGS58 were obtained. Although the issues of quantitative conversion of hydrogen from caffeine by the on-line HTC method have been investigated recently by Gehre et al. (2015) and Nair et al. (2015), further studies are required based on the results of the present study. Another observation from the data in Table 5 is that the pattern of mass fraction of hydrogen as function of particle size is different between USGS57 and USGS58 when analyzed in the same run. With the assumption that polyethylene does not suffer from hydrogen-conversion issues either with a glassy carbon-filled reactor or with a Cr-filled reactor, we decided to use the values of mass fraction of hydrogen for USGS57 and USGS58 derived using the reaction of polyethylene. The recommended mass fractions of hydrogen in USGS57 and USGS58 are 0.416% (3.74% as  $\text{H}_2\text{O}$ ) and 0.448% (4.03% as  $\text{H}_2\text{O}$ ), respectively (Table 5). These values agree well with the empirical mass fractions of hydrogen of 0.404% (3.64% as  $\text{H}_2\text{O}$ ) in biotite ( $\text{KMg}_{2.5}\text{Fe}_{0.5}^{2+}\text{AlSi}_3\text{O}_{10}(\text{OH})_{1.75}\text{F}_{0.25}$ ), and 0.451% (4.06% as  $\text{H}_2\text{O}$ ) in muscovite ( $\text{KAl}_3\text{Si}_3\text{O}_{10}(\text{OH})_{1.8}\text{F}_{0.2}$ ).

The mass fractions of hydrogen were also determined in the original material (200 to 300  $\mu\text{m}$ ) and the fine material (smaller than 74  $\mu\text{m}$ ) of NBS 30 by reaction of polyethylene in the same run with a glassy carbon reactor (Table 5). The mass fraction of hydrogen of 0.475% (4.27% as  $\text{H}_2\text{O}$ ) determined from the fine fraction is about 17% higher than that of value of 0.398% (3.55% as  $\text{H}_2\text{O}$ ) determined on the original material. This observation agrees well with the findings by Qi et al. (2014a). However, the water content of 4.27% in NBS 30 biotite is much too high compared to the empirical water content of 3.64% in pure biotite. We speculate that NBS 30 contains some impurities, such as lamellae of chlorite, with about 10–12% water by mass. This water cannot be released from the material having the original, relatively-large particle size by the on-line HTC method, but it can be released from the material with smaller particle size. The hydrogen yields from

different particle sizes of NBS 30 demonstrated a clear trend toward higher yield with finer grain size (Qi et al., 2014a). It is unclear how the assigned water content of 3.5% was obtained (Hut, 1987). We would assume that the manometry method would be used to determine the water content. Further study may be useful for investigating methods for accurate water content measurement.

#### 4.4. Moisture absorption and removal

To test the efficiency of water removal by drying samples of the RMs in a vacuum oven at 45 °C for few hours, a dual-water equilibration experiment was conducted. Results of this test were presented in Table 4 of Qi et al. (2014a). The sample named Biotite-1 (177  $\mu\text{m}$ ) is the same material as USGS57 and the sample named Muscovite-2 (149  $\mu\text{m}$ ) is USGS58. The two RMs were divided into three groups. The first group was analyzed without any treatment. The second group of samples was allowed to exchange with water vapor enriched in  $^2\text{H}$  (UC04 with  $\delta^2\text{H}_{\text{VSMOW-SLAP}} = +113 \text{ mUr}$ ). The third group of samples was allowed to exchange with water depleted in  $^2\text{H}$  (W-63333 with  $\delta^2\text{H}_{\text{VSMOW-SLAP}} = -399.5 \text{ mUr}$ ). The exchange experiment was conducted in a closed container at ambient temperature for 11 days. Samples were dried in a vacuum oven at 45 °C for 5 h prior to analysis. The  $\delta^2\text{H}$  values summarized in Table 6 indicate that neither the amount of water adsorbed on mineral surfaces, nor hydrogen isotopic exchange, are substantial at ambient temperature. The finer material, USGS58 muscovite, which was exposed to W-63333 had slightly more negative  $\delta^2\text{H}$  values, but values were within two sigma of the original material. The results in Table 6 confirm that there is little to no hydrogen exchange between hydrogen in two RMs and water at ambient temperature, and adsorbed moisture on both RMs can be removed effectively by drying in a vacuum oven at 45 °C for 5 h. The samples analyzed at the University of Oregon were all dried in vacuum at 130 °C for 14 h inside silver cups, immediately loaded (5 min exposure to air while in silver cups), and analyzed.

#### 4.5. The $\delta^2\text{H}_{\text{VSMOW-SLAP}}$ results

Six laboratories used on-line methods based on a variety of high temperature conversion elemental analyzers (HTC, with Cr-filled reactors or glassy carbon-filled reactors) and gas chromatographic (GC) interfaces, as well as mass spectrometers from different manufacturers (Table 1). The results (Table 7) are all normalized to the VSMOW-SLAP

**Table 6**

The  $\delta^2\text{H}$  values of USGS57 biotite and USGS58 muscovite.

[Each sample was divided into three groups. One group was analyzed without any treatment (labeled "Original"). The second group of samples was equilibrated in water enriched in  $^2\text{H}$ , UC04. The third group was equilibrated in water depleted in  $^2\text{H}$ , W-63333. The  $\delta^2\text{H}$  values are not normalized to the VSMOW-SLAP scale, but measured  $\delta^2\text{H}$  values are expressed relative to the same laboratory reference. Uncertainties are one standard deviation.]

Description	$\delta^2\text{H}$ (mUr)		
	USGS57 biotite	USGS58 muscovite	
	177 $\mu\text{m}$	149 $\mu\text{m}$	
Original	– 87.8	– 29.0	
	– 89.1	– 27.1	
	– 90.0	– 28.0	
Mean	– 89.0 $\pm$ 1.1	– 28.0 $\pm$ 1.0	
	Equilibrated with UC04	– 90.7	– 30.8
		– 92.1	– 28.8
– 90.9		– 28.6	
Mean	– 91.2 $\pm$ 0.8	– 29.4 $\pm$ 1.2	
	Equilibrated with W-63333	– 89.8	– 31.2
		– 89.1	– 30.1
– 92.8		– 30.2	
Mean	– 90.6 $\pm$ 2.0	– 30.5 $\pm$ 0.6	

**Table 7**

The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of USGS57 biotite, USGS58 muscovite, and NBS 30 biotite isotopic reference materials analyzed by on-line high temperature conversion/elemental analyzer and an off-line method by seven isotope laboratories.

[Uncertainties are one-sigma standard deviations.]

Laboratory	Run #	Reactor type	Condition	USGS57 biotite		USGS58 muscovite		NBS 30 biotite	
				$\delta^2\text{H}_{\text{VSMOW-SLAP}}$ (mUr)	<i>n</i>	$\delta^2\text{H}_{\text{VSMOW-SLAP}}$ (mUr)	<i>n</i>	$\delta^2\text{H}_{\text{VSMOW-SLAP}}$ (mUr)	<i>n</i>
UC	1	Glassy carbon	1450 °C	-94.7 ± 1.0	11	-29.9 ± 1.3	12	-54.0 ± 1.7	4
UL	1	Glassy carbon	1450 °C	-89.4 ± 1.0	10	-25.7 ± 1.0	10	-47.7 ± 3.5	7
UO	1	Glassy carbon	1450 °C	-92.3 ± 1.3	3	-30.6 ± 0.6	3	-57.0 ± 1.0	3
UO	2	Glassy carbon	1450 °C	-91.0 ± 0.6	3	-28.0 ± 0.5	3	-54.3 ± 1.6	3
UO	3	Glassy carbon	1450 °C	-91.0 ± 1.2	4	-28.0 ± 1.8	4	-54.0 ± 1.7	4
UO	4	Glassy carbon	1450 °C	-95.2 ± 0.4	3	-31.2 ± 0.1	3	-54.0 ± 1.7	3
UO	5	Glassy carbon	1450 °C	-95.6 ± 0.1	2	-32.7 ± 0.7	2	-54.0 ± 1.7	3
UO	6	Glassy carbon	1450 °C	-91.0 ± 1.2	4	-28.1 ± 1.4	4	-54.0 ± 1.7	4
UFZ	1	Cr	1150 °C	-86.8 ± 1.7	5	-27.8 ± 0.1	5	-53.1 ± 0.5	5
UFZ	2	Cr	1150 °C	-86.5 ± 2.1	5	-27.8 ± 0.5	5	-53.0 ± 0.4	5
UFZ	3	Cr	1270 °C	-91.9 ± 1.3	5	-29.9 ± 0.6	5	-54.1 ± 0.8	5
UFZ	4	Cr	1270 °C	-93.4 ± 0.9	4	-30.0 ± 0.8	4	-54.1 ± 0.7	4
UFZ	5	Cr	1270 °C with V <sub>2</sub> O <sub>5</sub>	-89.0 ± 0.7	4	-27.3 ± 0.9	4	-51.9 ± 1.3	5
UFZ	6	Cr	1270 °C with V <sub>2</sub> O <sub>5</sub>	-90.1 ± 1.5	5	-27.2 ± 2.6	4	-51.0 ± 1.0	5
UFZ	7	Cr	1270 °C with V <sub>2</sub> O <sub>5</sub> + O <sub>2</sub>	-89.6 ± 1.3	5	-28.4 ± 1.0	5	-52.3 ± 0.9	5
MPI-BGC	1	Cr	1430 °C	-91.1 ± 0.5	4	-27.4 ± 0.6	4	-52.3 ± 0.4	4
MPI-BGC	2	Cr	1400 °C	-91.2 ± 0.7	4	-26.5 ± 0.5	4	-52.3 ± 1.3	4
MPI-BGC	3	Cr	1400 °C	-93.7 ± 0.7	4	-28.2 ± 0.4	4	-53.8 ± 0.8	4
RSIL	1	Glassy carbon	1450 °C	-89.5 ± 0.7	7	-26.2 ± 1.5	7	-49.5 ± 1.2	7
RSIL	2	Cr	1050 °C	-91.9 ± 1.1	6	-28.8 ± 0.3	6	-53.8 ± 0.6	6
RSIL	3	Cr	1050 °C to 1350 °C <sup>a</sup>	-92.4 ± 0.9	7	-27.6 ± 0.6	7	-54.2 ± 1.1	7
RSIL	4	Cr	1050 °C	-92.5 ± 0.6	7	-28.0 ± 0.8	5	-54.9 ± 1.2	6
RSIL	5	Cr	1150 °C	-94.2 ± 2.0	3	-27.5 ± 0.3	3	-55.1 ± 1.2	3
UWO	Average on-line data			-91.5 ± 2.4, <i>n</i> = 23		-28.4 ± 1.7, <i>n</i> = 23		-53.4 ± 2.5, <i>n</i> = 23	
	Off-line <sup>b</sup>			-92.9 ± 2.8	5	-28.1 ± 0.8	5		
	Average all			-91.5 ± 2.4, <i>n</i> = 24		-28.4 ± 1.6, <i>n</i> = 24			

<sup>a</sup> Each sample was analyzed at different temperatures between 1050 °C and 1350 °C.

<sup>b</sup> The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  measurements determined with the off-line method were performed on different days.

scale using two-point calibration. The average  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of  $-91.5 \pm 2.4$  mUr for USGS57 biotite and  $-28.4 \pm 1.7$  mUr for USGS58 muscovite analyzed by six laboratories using on-line HTC methods (both glassy carbon-filled reactors and Cr-filled reactors) were confirmed by the results obtained using the off-line method ( $-92.9 \pm 2.8$  mUr for USGS57 and  $-28.1 \pm 0.8$  mUr for USGS58). The final mean  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of  $-91.5 \pm 2.4$  mUr for USGS57 biotite and  $-28.4 \pm 1.6$  mUr for USGS58 muscovite were calculated from 23 on-line results and one off-line result. The uncertainties are given as 1- $\sigma$  standard deviations.

The UFZ, MPI-BGC, and RSIL performed measurements at different temperatures using Cr-filled reactors with temperatures ranging between 1050 °C and 1430 °C; no systematic difference was observed within analytical uncertainty. A typical  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  measurement uncertainty was  $\sim 1$  to 2 mUr. Although variations in  $\delta^2\text{H}$  values and hydrogen yields from samples with different particle sizes of USGS57 and USGS58 were observed using both a glassy carbon-filled reactor and a Cr-filled reactor (as discussed early), one would assume that the measured  $\delta^2\text{H}$  values with highest hydrogen yields should be considered as the most reliable values. However, the overall uncertainties of  $\delta^2\text{H}$  values from all size fractions (Table 4) are insignificant compare to the measurement results shown in Table 7. The average uncertainties of  $\delta^2\text{H}$  values from all size fractions are in the range of 0.3 to 1.2 mUr for USGS57 and 1.9 to 2.7 mUr for USGS58, respectively (Table 4).

The mean  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  value of  $-53.4 \pm 2.5$  mUr for NBS 30 biotite obtained from 9 analyses using a glassy carbon-filled reactor and 14 analyses using a Cr-filled reactor (at different temperatures) by five laboratories confirmed the findings of Qi et al. (2014a) that the  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of NBS 30 biotite (having an original particle size between 200 and 300  $\mu\text{m}$ ) analyzed by on-line HTC systems can be substantially too positive compared to the accepted value of  $-65.7$  mUr (Gonfiantini et al., 1995). Although USGS57 is biotite, it behaves differently in the HTC systems than NBS 30 biotite because

USGS57 biotite contains fewer impurities than NBS 30. Unlike NBS 30, USGS57 is homogeneous among the size fractions analyzed and does not contain an alteration product (chlorite) in its final fractions. The conversion of hydroxyl ions in USGS58 muscovite to molecular hydrogen is hypothesized to be quantitative. Users should be cautious in analyzing hydrous minerals using on-line HTC systems. Conversion of hydrogen in minerals to molecular hydrogen may not be quantitative, depending upon their chemical composition and particle size, even for the same phase (e.g. biotite) with the result that  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values may be unreliable.

#### 4.6. Additional observation with caffeine

To quantify accurately the mass fraction of hydrogen in the two RMs, several aliquots of USGS62 caffeine with precisely determined (and different) masses were analyzed at the beginning, middle, and end of a run to monitor and adjust for apparent changes in the hydrogen yield during a run using both a glassy carbon-filled reactor and a Cr-filled reactor. The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  results and relative hydrogen yields (expressed as relative hydrogen peak area / mass) are summarized in Table 8.

Caffeine samples placed at the beginning of a sequence were analyzed with a newly packed glassy carbon reactor. As one might expect, formation of hydrogen-bearing by-products (HCN) from the caffeine reaction prevent quantitative conversion of organic hydrogen to molecular hydrogen when a conventional on-line HTC method with a glassy carbon-filled reactor is used. Thus,  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  results are seriously compromised due to non-quantitative conversion of hydrogen to molecular hydrogen (Gehre et al., 2015). This is demonstrated in Fig. 2a with data obtained from a newly packed reactor. The caffeine samples at the middle of the sequence were analyzed after 20 biotite samples having 3.5-mg samples. The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values and relative hydrogen yields from caffeine changed from  $-175.2$  mUr (analyzed in



**Table 8**

The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values and relative hydrogen yields (relative peak area / mass) of caffeine (USGS62) analyzed by a glassy carbon-filled reactor and a Cr-filled reactor. [Uncertainties are one-sigma standard deviations. Each data point is the mean value of two to three analyses.]

	Glassy carbon-filled reactor		Cr-filled reactor	
	$\delta^2\text{H}_{\text{VSMOW-SLAP}}$ (mUr)	Relative H <sub>2</sub> yield	$\delta^2\text{H}_{\text{VSMOW-SLAP}}$ (mUr)	Relative H <sub>2</sub> yield
Fresh reactor	$-175.5 \pm 0.5$	$132.2 \pm 2.8$	$-153.3 \pm 2.0$	$210.7 \pm 6.4$
After biotite	$-166.5 \pm 1.7$	$156.0 \pm 3.6$	$-154.7 \pm 0.1$	$211.3 \pm 3.0$
After muscovite	$-158.4 \pm 2.2$	$178.0 \pm 5.5$	$-154.3 \pm 0.5$	$211.4 \pm 11.0$

fresh reactor) to  $-166.5$  mUr (analyzed after biotite), and 132 (analyzed in fresh reactor) to 156 (analyzed after biotite), respectively (Fig. 2a). The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values of  $-158.4 \pm 2.2$  mUr from caffeine analyzed at end of the sequence of 20 muscovite samples is almost identical to the assigned value of  $-156.1 \pm 2.1$  mUr (Schimmelmann et al., 2016). The relative hydrogen yield also increased substantially. This observation indicates that the mineral residue generated from high temperature conversion can prevent formation of HCN from caffeine and can improve quantitative conversion of hydrogen. Analysis with an identical arrangement of samples in the sequence was carried out with a Cr-filled reactor. Both  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values and relative hydrogen yields from caffeine were approximately the same throughout the sequence (Fig. 2b). From these observations, one needs to be cautious in deciding whether glassy carbon-filled or Cr-filled reactors should be used when different materials are included in the same analytical sequence.

## 5. Conclusion

The supply of the internationally distributed isotopic reference material NBS 30 biotite is exhausted. To ensure accurate and traceable on-line hydrogen isotope-ratio determinations of mineral samples, two isotopically homogeneous hydrous mineral RMs, USGS57 biotite and USGS58 muscovite (available in amounts of 0.5 g in a glass vial) have been prepared by the U.S. Geological Survey (<http://isotopes.usgs.gov/lab/referencematerials.html>). The  $\delta^2\text{H}$  values were determined by both glassy carbon-based on-line conversion and chromium-based on-line conversion by six international isotope laboratories, and results were verified by the classic off-line conversion technique. Isotopic compositions with 1- $\sigma$  uncertainties and mass fractions of hydrogen in these materials are:

USGS57 (biotite)

$\delta^2\text{H}_{\text{VSMOW-SLAP}} = -91.5 \pm 2.4$  mUr ( $n = 24$ )

Hydrogen mass fraction =  $0.416 \pm 0.002\%$  ( $n = 4$ )

Fraction of water =  $3.74 \pm 0.02\%$  ( $n = 4$ )

USGS58 (muscovite)

$\delta^2\text{H}_{\text{VSMOW-SLAP}} = -28.4 \pm 1.6$  mUr ( $n = 24$ )

Hydrogen mass fraction =  $0.448 \pm 0.002\%$  ( $n = 4$ )

Fraction of water =  $4.03 \pm 0.02\%$  ( $n = 4$ ).

The use of these RMs enables high quality and standardized stable isotope measurements of hydrogen in hydrous mineral samples. Analyzing a mineral sample with a particle size  $\leq 74 \mu\text{m}$  and  $\geq 177 \mu\text{m}$  is not recommended based on this study. Users should be cautious in analyzing hydrous minerals with on-line HTC systems because conversion of hydrogen in minerals to molecular hydrogen may not be quantitative, depending upon mineral chemical composition (e.g. higher iron content) and particle size. There is no significant difference in results for these two RMs between samples analyzed using the glassy carbon-filled reactor method or the Cr-filled reactor method. The glassy carbon-based conversion method yields more consistent  $\delta^2\text{H}$  values than the Cr-based conversion for the two RMs, especially for USGS57 biotite. Further study may be needed for investigating the accurate water content of NBS 30 biotite.

## Acknowledgements

We thank Daniel M. Webster (U.S. Geological Survey, retired) for analyzing samples by X-ray diffraction measurements. We thank Grace Yau for analyzing hydrogen isotopes by an off-line method at The University of Western Ontario, Canada. This manuscript benefited from careful reviews by John A. Mering (University of Waikato, New Zealand) and two anonymous reviewers. The support of the U.S. Geological Survey National Research Program made this article possible. The University of Chicago equipment was supported in part by NSF award #0923831, funded under the American Recovery and Reinvestment Act of 2009 (Public Law 111-5). Support was also provided by the Natural Sciences and Engineering Research Council of Canada (FJL) (05293-2014 RGPIN), the Canada Foundation for

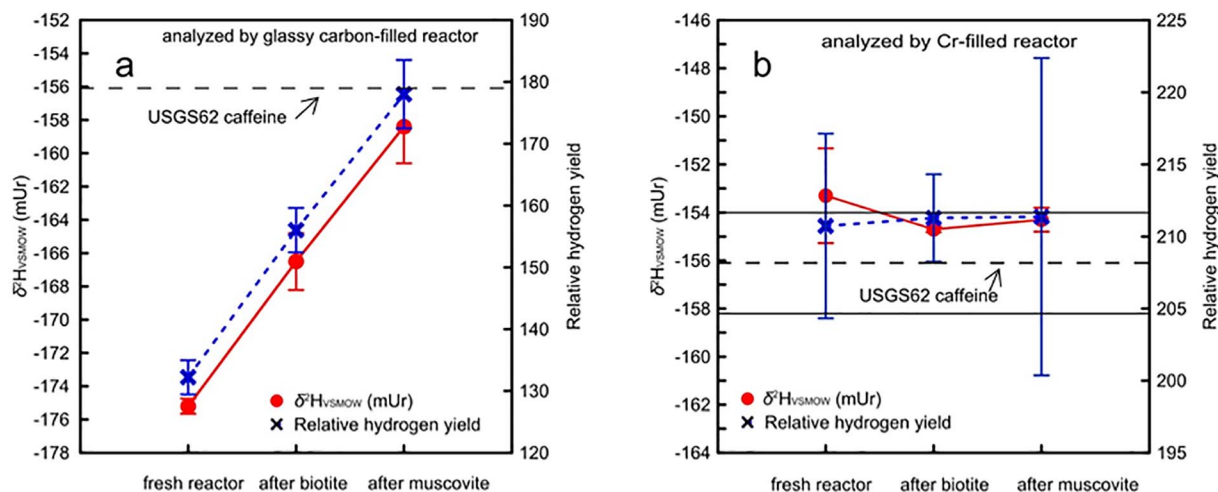


Fig. 2. The  $\delta^2\text{H}_{\text{VSMOW-SLAP}}$  values and relative hydrogen yields (relative peak areas / mass) of USGS62 caffeine analyzed at the beginning (fresh reactor), middle (after biotite), and end (after muscovite) of a sequence using a glassy carbon-filled reactor (a) and a Cr-filled reactor (b).

Innovation (FJL) (2732), and the Canada Research Chairs program (FJL) (950-226925). This is Western's Laboratory for Stable Isotope Science (LSIS) Contribution #349. Any use of trade, firm, or product names is for descriptive purposes only and does not imply endorsement by the U.S. Government.

## References

- Abruzzese, M.J., Waldbauer, J.R., Chamberlain, C.P., 2005. Oxygen and hydrogen isotope ratios in freshwater chert as indicators of ancient climate and hydrologic regime. *Geochim. Cosmochim. Acta* 69 (6), 1377–1390. <http://dx.doi.org/10.1016/j.gca.2004.08.036>.
- Alexander, C.M.O'D., Howard, K.T., Bowden, R., Fogel, M.L., 2013. The classification of CM and CR chondrites using bulk H, C and N abundances and isotopic compositions. *Geochim. Cosmochim. Acta* 123, 244–260. <http://dx.doi.org/10.1016/j.gca.2013.05.019>.
- Armbruster, W., Lehnert, K., Vetter, W., 2006. Establishing a chromium-reactor design for measuring  $\delta^2\text{H}$  values of solid polyhalogenated compounds using direct elemental analysis and stable isotope ratio mass spectrometry. *Anal. Bioanal. Chem.* 384, 237–243. <http://dx.doi.org/10.1007/s00216-005-0160-0>.
- Bauer, K.K., Vennemann, T.W., 2014. Analytical methods for the measurement of hydrogen isotope composition and water content in clay minerals by TC/EA. *Chem. Geol.* 363, 229–240. <http://dx.doi.org/10.1016/j.chemgeo.2013.10.039>.
- Begley, I.S., Scrimgeour, C.M., 1996. On-line reduction of  $\text{H}_2\text{O}$  for  $\delta^2\text{H}$  and  $\delta^{18}\text{O}$  measurement by continuous-flow isotope ratio mass spectrometry. *Rapid Commun. Mass Spectrom.* 10, 969–973. [http://dx.doi.org/10.1002/\(SICI\)1097-0231\(19960610\)10:8<969::AID-RCM532>3.0.CO;2-O](http://dx.doi.org/10.1002/(SICI)1097-0231(19960610)10:8<969::AID-RCM532>3.0.CO;2-O).
- Bigeleisen, J., Perlman, M.L., Prosser, H.C., 1952. Conversion of hydrogenic materials to hydrogen for isotopic analysis. *Anal. Chem.* 24, 1356–1357. <http://dx.doi.org/10.1021/ac60068a025>.
- Bindeman, I.N., Kamenetsky, V.S., Palandri, J., Vennemann, T., 2012. Hydrogen and oxygen isotope behaviors during variable degrees of upper mantle melting: example from the basaltic glass from Macquarie Island. *Chem. Geol.* 310–311, 126–136. <http://dx.doi.org/10.1016/j.chemgeo.2012.03.031>.
- Brand, W.A., Coplen, T.B., 2012. Stable isotope deltas: tiny, yet robust signatures in nature. *Isot. Environ. Health Stud.* 48, 393–409. <http://dx.doi.org/10.1080/10256016.2012.666977>.
- Brand, W.A., Coplen, T.B., Vogl, J., Rosner, M., Prohaska, T., 2014. Assessment of international reference materials for isotope-ratio analysis (IUPAC technical report). *Pure Appl. Chem.* 86, 425–467. <http://dx.doi.org/10.1515/pac-2013-1023>.
- Burgoyne, T.W., Hayes, J.M., 1998. Quantitative production of  $\text{H}_2$  by pyrolysis of gas chromatographic effluents. *Anal. Chem.* 70, 5136–5141. <http://dx.doi.org/10.1021/ac980248v>.
- Cohen, E.R., Cvitaš, T., Holmström, B., Kuchitsu, K., Marquardt, R., Mills, I., Pavese, F., Quack, M., Stohner, J., Strauss, H.L., Takami, M., Thor, A.J., 2007. Quantities, Units and Symbols in Physical Chemistry. RSC Publishing, Cambridge, UK 234 p. [https://www.iupac.org/fileadmin/user\\_upload/publications/e-resources/ONLINE-IUPAC-GB3-2ndPrinting-Online-Sep2012.pdf](https://www.iupac.org/fileadmin/user_upload/publications/e-resources/ONLINE-IUPAC-GB3-2ndPrinting-Online-Sep2012.pdf).
- Coleman, M.L., Shepherd, T.J., Durham, J.J., Rouse, J.E., Moore, G.R., 1982. Reduction of water with zinc for hydrogen isotope analysis. *Anal. Chem.* 54, 993–995. <http://dx.doi.org/10.1021/ac00243a035>.
- Coplen, T.B., 1988. Normalization of oxygen and hydrogen isotope data. *Chem. Geol. (Isotope Geosci. Sec.)* 72, 293–297. [http://dx.doi.org/10.1016/0168-9622\(88\)90042-5](http://dx.doi.org/10.1016/0168-9622(88)90042-5).
- Coplen, T.B., 1994. Reporting of stable hydrogen, carbon, and oxygen isotopic abundances. *Pure Appl. Chem.* 66, 273–276. <http://dx.doi.org/10.1351/pac199466020273>.
- Coplen, T.B., 1996. New guidelines for the reporting of stable hydrogen, carbon, and oxygen isotope-ratio data. *Geochim. Cosmochim. Acta* 60, 3359–3360. [http://dx.doi.org/10.1016/0016-7037\(96\)00263-3](http://dx.doi.org/10.1016/0016-7037(96)00263-3).
- Coplen, T.B., 2011. Guidelines and recommended terms for expression of stable-isotope-ratio and gas-ratio measurement results. *Rapid Commun. Mass Spectrom.* 25, 2538–2560. <http://onlinelibrary.wiley.com/doi/10.1002/rcm.5129/abstract>.
- Coplen, T.B., Qi, H., 2010. Applying the silver-tube introduction method for thermal conversion elemental analyses and a new  $\delta^2\text{H}$  value for NBS 22 oil. *Rapid Commun. Mass Spectrom.* 24, 2269–2276. <http://dx.doi.org/10.1002/rcm.4638>.
- Coplen, T.B., Qi, H., 2016. A revision in hydrogen isotopic composition of USGS42 and USGS43 human-hair stable isotopic reference materials for forensic science. *Forens. Sci. Intern.* 266, 222–225. <http://dx.doi.org/10.1016/j.forsciint.2016.05.029>.
- Deering, C.D., Horton, T.W., Gravley, D.M., Cole, J.W., 2012. Hornblende, cummingtonite, and biotite hydrogen isotopes: direct evidence of slab-derived fluid flux in silicic magmas of the Taupo Volcanic Zone, New Zealand. *J. Volcanol. Geotherm. Res.* 233–234, 27–36. <http://dx.doi.org/10.1016/j.jvolgeores.2012.04.010>.
- Friedman, I., 1953. Deuterium content of natural water and other substances. *Geochim. Cosmochim. Acta* 4, 89–103. [http://dx.doi.org/10.1016/0016-7037\(53\)90066-0](http://dx.doi.org/10.1016/0016-7037(53)90066-0).
- Gehre, M., Geilmann, H., Richter, J., Werner, R.A., Brand, W.A., 2004. Continuous flow  $^2\text{H}/^1\text{H}$  and  $^{18}\text{O}/^{16}\text{O}$  analysis of water samples with dual inlet precision. *Rapid Commun. Mass Spectrom.* 18, 2650–2660.
- Gehre, M., Renpenning, J., Gilevska, T., Qi, H., Coplen, T.B., Meijer, H.A.J., Brand, W.A., Schimmelmann, A., 2015. On-line hydrogen-isotope measurements of organic samples using elemental chromium—an extension for high temperature elemental analyzer techniques. *Anal. Chem.* 87, 5198–5205. <http://dx.doi.org/10.1021/acs.analchem.5b00085>.
- Gehre, M., Renpenning, J., Geilmann, H., Qi, H., Coplen, T.B., Kümmel, S., Ivdrá, N., Brand, W.A., Schimmelmann, A., 2017. Optimization of on-line hydrogen stable isotope-ratio measurements of halogen- and sulfur-bearing organic compounds using elemental analyzer-chromium/high-temperature conversion (EA–Cr/HTC–IRMS). *Rapid Commun. Mass Spectrom.* 31, 475–484. <http://dx.doi.org/10.1002/rcm.7810>.
- Godfrey, J.D., 1962. The deuterium content of hydrous minerals from the East-Central Sierra Nevada and Yosemite National Park. *Geochim. Cosmochim. Acta* 26, 1215–1245. [http://dx.doi.org/10.1016/0016-7037\(62\)90053-4](http://dx.doi.org/10.1016/0016-7037(62)90053-4).
- Gonfiantini, R., 1978. Standards for stable isotope measurements in natural compounds. *Nature* 271, 534–536. <http://dx.doi.org/10.1038/271534a0>.
- Gonfiantini, R., 1984. Advisory Group meeting on stable isotope reference samples for geochemical and hydrological investigations. In: Report to the Director General. International Atomic Energy Agency. [http://www.naweb.iaea.org/NAALIH/docs/pub/IAEA-1984-Gonfiantini\\_AGMeeting-StableisotopeRM.pdf](http://www.naweb.iaea.org/NAALIH/docs/pub/IAEA-1984-Gonfiantini_AGMeeting-StableisotopeRM.pdf).
- Gonfiantini, R., Stiehler, W., Rozanski, K., 1995. Standards and intercomparison materials distributed by the International Atomic Energy Agency. In: Reference and Intercomparison Materials for Stable Isotopes of Light Elements. International Atomic Energy Agency, pp. 13. IAEA-TECDOC-825. [http://www-pub.iaea.org/MTCD/Publications/PDF/te\\_825\\_prn.pdf](http://www-pub.iaea.org/MTCD/Publications/PDF/te_825_prn.pdf).
- Gong, B., Zheng, Y.-F., Chen, R.-X., 2007. An online method combining a thermal conversion elemental analyzer with isotope ratio mass spectrometry for the determination of hydrogen isotope composition and water concentration in geological samples. *Rapid Commun. Mass Spectrom.* 21, 1386–1392. <http://dx.doi.org/10.1002/rcm.2973>.
- Hilkert, A.W., Douthitt, C.B., Schlüter, H.J., Brand, W.A., 1999. Isotope ratio monitoring gas chromatography/mass spectrometry of D/H by high temperature conversion isotope ratio mass spectrometry. *Rapid Commun. Mass Spectrom.* 13, 1226–1230. [http://dx.doi.org/10.1002/\(SICI\)1097-0231\(19990715\)13:13<1226::AID-RCM575>3.0.CO;2-9](http://dx.doi.org/10.1002/(SICI)1097-0231(19990715)13:13<1226::AID-RCM575>3.0.CO;2-9).
- Hunsinger, G.B., Tipple, C.A., Stern, L.A., 2013. Gaseous byproducts from high-temperature thermal conversion elemental analysis of nitrogen- and sulfur-bearing compounds with considerations for  $\delta^2\text{H}$  and  $\delta^{18}\text{O}$  analyses. *Rapid Commun. Mass Spectrom.* 27, 1649–1659. <http://dx.doi.org/10.1002/rcm.6608>.
- Hut, G., 1987. Consultants' group meeting on stable isotope reference samples for geochemical and hydrological investigations. In: Report to the Director General. International Atomic Energy Agency, Vienna. <http://www.iaea.org/inis/collection/NCLCollectionStore/Public/18/075/180755746.pdf>.
- Kendall, C., Coplen, T.B., 1985. Multisample conversion of water to hydrogen by zinc for stable isotope determination. *Anal. Chem.* 57, 1437–1440.
- Kokubu, N., Mayeda, T., Urey, H.C., 1961. Deuterium content of minerals, rocks and liquid inclusions from rocks. *Geochim. Cosmochim. Acta* 21, 247–256. [http://dx.doi.org/10.1016/S0016-7037\(61\)80058-6](http://dx.doi.org/10.1016/S0016-7037(61)80058-6).
- Kyser, T.K., O'Neil, J.R., 1984. Hydrogen isotope systematics of submarine basalts. *Geochim. Cosmochim. Acta* 48, 2123–2133. [http://dx.doi.org/10.1016/0016-7037\(84\)90392-2](http://dx.doi.org/10.1016/0016-7037(84)90392-2).
- Marks, M., Vennemann, T., Siebel, W., Markl, G., 2004. Nd-, O-, and H-isotopic evidence for complex, closed-system fluid evolution of the peralkaline Ilímaussaq intrusion, south Greenland. *Geochim. Cosmochim. Acta* 68 (16), 3379–3395. <http://dx.doi.org/10.1016/j.gca.2003.12.008>.
- Martin, E., Bindeman, I.N., Balan, E., Palandri, J., Seligman, A., Villemant, B., 2017. Hydrogen isotope determination by TC/EA technique in application to volcanic glass as a window into secondary hydration. *J. Volcanol. Geoth. Res. (In press)*.
- Mittempergher, S., Dallai, L., Pennacchioni, G., Renard, F., Di Toro, G., 2014. Origin of hydrogen fluids at seismogenic depth: constraints from natural and experimental fault rocks. *Earth Planet. Sci. Lett.* 385, 97–109. <http://dx.doi.org/10.1016/j.epsl.2013.10.027>.
- Nair, S., Geilmann, H., Coplen, T.B., Qi, H., Gehre, M., 2015. Isotopic disproportionation during hydrogen isotopic analysis of nitrogen-bearing organic compounds. *Rapid Commun. Mass Spectrom.* 29, 878–884. <http://dx.doi.org/10.1002/rcm.7174>.
- Paul, D., Skrzypek, G., Foriz, I., 2007. Normalization of measured stable isotopic compositions to isotope reference scales—a review. *Rapid Commun. Mass Spectrom.* 21, 3006–3014. <http://dx.doi.org/10.1002/rcm.3185>.
- Qi, H., Gröning, M., Coplen, T.B., Buck, B., Mroczkowski, S.J., Brand, W.A., Geilmann, H., Gehre, M., 2010. Novel silver-tubing method for quantitative introduction of water into high-temperature conversion systems for stable hydrogen and oxygen isotopic measurements. *Rapid Commun. Mass Spectrom.* 24, 1821–1827. <http://dx.doi.org/10.1002/rcm.4559>.
- Qi, H., Coplen, T.B., Olack, G., Vennemann, T.W., 2014a. Caution on the use of NBS 30 biotite for hydrogen-isotope measurements with on-line high-temperature conversion systems. *Rapid Commun. Mass Spectrom.* 28, 1987–1994. <http://dx.doi.org/10.1002/rcm.6983>.
- Qi, H., Lorenz, J., Coplen, T.B., Tarbox, L., Mayer, B., Taylor, S., 2014b. Lake Louise Water (USGS47): a new isotopic reference water for stable hydrogen and oxygen isotope measurements. *Rapid Commun. Mass Spectrom.* 28, 351–354. <http://dx.doi.org/10.1002/rcm.6789>.
- Savin, S.M., Epstein, S., 1970. The oxygen and hydrogen isotope geochemistry of clay minerals. *Geochim. Cosmochim. Acta* 34, 25–42. [http://dx.doi.org/10.1016/0016-7037\(70\)90149-3](http://dx.doi.org/10.1016/0016-7037(70)90149-3).
- Schimmelmann, A., Albertino, A., Sauer, P.E., Qi, H., Molinie, R., Mesnard, F., 2009. Nicotine, acetanilide and urea multi-level  $^2\text{H}$ -,  $^{13}\text{C}$ - and  $^{15}\text{N}$ -abundance reference materials for continuous-flow isotope ratio mass spectrometry. *Rapid Commun. Mass Spectrom.* 23, 3513–3521. <http://dx.doi.org/10.1002/rcm.4277>.
- Schimmelmann, A., Qi, H., Coplen, T.B., Brand, W.A., Fong, J., Meier-Augenstein, W., Kemp, H.F., Toman, B., Ackermann, A., Assonov, S., Aerts-Bijma, A.T., Brejcha, R., Chikaraish, Y., Darwish, T., Elsnar, M., Gehre, M., Geilmann, H., Gröning, M., Hélie, J.-F., Herrero-Martín, S., Meijer, H.A.J., Sauer, P.E., Sessions, A.L., Werner, R.A.,

2016. Organic reference materials for hydrogen, carbon, and nitrogen stable isotope-ratio measurements: caffeine, n-alkanes, fatty acid, methyl esters, glycines, L-valines, polyethylenes, and oils. *Anal. Chem.* 88, 4294–4302. <http://dx.doi.org/10.1021/acs.analchem.5b04392>.
- Seligman, A.N., Bindeman, I.N., Watkins, J.M., Ross, A.M., 2016. Water in volcanic glass: from volcanic degassing to secondary hydration. *Geochim. Cosmochim. Acta* 191, 216–238. <http://dx.doi.org/10.1016/j.gca.2016.07.010>.
- Sharp, Z.D., Atudorei, V., Durakiewicz, T., 2001. A rapid method for determination of hydrogen and oxygen isotope ratios from water and hydrous minerals. *Chem. Geol.* 178, 197–210. [http://dx.doi.org/10.1016/S0009-2541\(01\)00262-5](http://dx.doi.org/10.1016/S0009-2541(01)00262-5).
- Suzuoki, T., Epstein, S., 1976. Hydrogen isotope fractionation between OH-bearing minerals and water. *Geochim. Cosmochim. Acta* 40, 1229–1240. [http://dx.doi.org/10.1016/0016-7037\(76\)90158-7](http://dx.doi.org/10.1016/0016-7037(76)90158-7).
- Underwood, S.J., Feeley, T.C., Clynne, M.A., 2012. Hydrogen isotope investigation of amphibole and biotite phenocrysts in silicic magmas erupted at Lassen Volcanic Center, California. *J. Volcanol. Geoth. Res.* 227–228, 32–49. <http://dx.doi.org/10.1016/j.jvolgeores.2012.02.019>.
- VanDeVelde, J.H., Bowen, G.J., 2013. Effects of chemical pretreatments on the hydrogen isotope composition of 2:1 clay minerals. *Rapid Commun. Mass Spectrom.* 27, 1143–1148. <http://dx.doi.org/10.1002/rcm.6554>.
- Vennemann, T.W., O'Neil, J.R., 1993. A simple and inexpensive method of hydrogen isotope and water analyses of minerals and rocks based on zinc reagent. *Chem. Geol. (Isotope Geosci. Sec.)* 103, 227–234. [http://dx.doi.org/10.1016/0009-2541\(93\)90303-Z](http://dx.doi.org/10.1016/0009-2541(93)90303-Z).
- Werner, R.A., Brand, W.A., 2001. Referencing strategies and techniques in stable isotope ratio analysis. *Rapid Commun. Mass Spectrom.* 15, 501–519. <http://dx.doi.org/10.1002/rcm.258>.