

**Serveur Académique Lausannois SERVAL [serval.unil.ch](http://serval.unil.ch)**

## **Author Manuscript**

**Faculty of Biology and Medicine Publication**

**This paper has been peer-reviewed but does not include the final publisher proof-corrections or journal pagination.**

Published in final edited form as:

**Title:** Development of a new chlamydiales-specific real-time PCR and its application to respiratory clinical samples.

**Authors:** Lienard J, Croxatto A, Aeby S, Jatton K, Posfay-Barbe K, Gervaix A, Greub G

**Journal:** Journal of clinical microbiology

**Year:** 2011 Jul

**Volume:** 49

**Issue:** 7

**Pages:** 2637-42

**DOI:** 10.1128/JCM.00114-11

In the absence of a copyright statement, users should assume that standard copyright protection applies, unless the article contains an explicit statement to the contrary. In case of doubt, contact the journal publisher to verify the copyright status of an article.

**Development of a new *Chlamydiales*-specific real-time PCR and its application to respiratory clinical samples**

Julia Lienard<sup>1</sup>, Antony Croxatto<sup>1</sup>, Sebastien Aeby<sup>1</sup>, Katia Jatton<sup>1</sup>, Klara Posfay-Barbe<sup>2</sup>, Alain Gervais<sup>2</sup> and Gilbert Greub<sup>1\*</sup>

<sup>1</sup>Institute of Microbiology, University Hospital Center and University of Lausanne, Lausanne, Switzerland.

<sup>2</sup>Children's Hospital of Geneva, University Hospitals of Geneva, Geneva, Switzerland

**Corresponding author:**

**\*Gilbert Greub, MD PhD**

Center for Research on Intracellular Bacteria (CRIB),

Institute of Microbiology, University Hospital Center and University of Lausanne,

1011 Lausanne

SWITZERLAND

Phone : +41-21-314 49 79

Fax : +41-21-314 40 60

E-mail : gilbert.greub@chuv.ch

**Running title:** New *Chlamydiales*-specific PCR

Word count of the main text: 3163 words

Word count of the abstract: 221 words

Keywords: new species, *Chlamydiales*, taxonomy, obligate intracellular bacteria

## Abstract

1 Originally composed of the single family *Chlamydiaceae*, the *Chlamydiales* order has  
2 extended considerably in the last decades. *Chlamydia*-related bacteria were added and  
3 classified in 6 different families and family-level lineages: the *Criblamydiaceae*,  
4 *Parachlamydiaceae*, *Piscichlamydiaceae*, *Rabdochlamydiaceae*, *Simkaniaceae* and  
5 *Waddliaceae*. While several members of the *Chlamydiaceae* family are known pathogens,  
6 recent studies showed diverse associations of *Chlamydia*-related bacteria with human and  
7 animal infections. Some of these latter bacteria are preoccupying since, given their ability to  
8 replicate in free-living amoebae, they may also replicate efficiently in other phagocytic cells,  
9 including cells of the innate immune system. Thus, a new *Chlamydiales*-specific real-time  
10 PCR targeting the conserved 16S rRNA gene was developed. This new molecular tool can  
11 detect at least 5 DNA copies and show very high specificity without cross-amplification  
12 from other bacterial clade DNA. The new PCR was validated with 128 clinical samples  
13 positive or negative for *Chlamydia trachomatis* or *C. pneumoniae*. Among 65 positive  
14 samples, 61 (93.8%) were found positive with the new PCR. The 4 discordant samples, re-  
15 tested with the original test, were negative or below detection limits. Then, the new PCR  
16 was applied to 422 nasopharyngeal swabs taken from children with and without  
17 pneumonia: 48 (11.4%) samples were positive, of which 45 were successfully sequenced.  
18 The majority of the sequences corresponded to *Chlamydia*-related bacteria and especially to  
19 members of the *Parachlamydiaceae* family.

20

21 INTRODUCTION

22 The *Chlamydiales* order contains obligate intracellular bacteria separated in 7 different  
23 families and family-level lineages, the *Chlamydiaceae*, the *Criblamydiaceae*, the  
24 *Parachlamydiaceae*, the *Piscichlamydiaceae*, the *Rhabdochlamydiaceae*, the *Simkaniaceae*  
25 and the *Waddliaceae* (16, 23-25). Some of these bacteria are established pathogens and for  
26 instance, *Chlamydia trachomatis*, *C. psittaci* and *C. pneumoniae* from the *Chlamydiaceae*  
27 family can cause significant human infections. The others families constitute a group called  
28 *Chlamydia*-related bacteria (also referred as *Chlamydia*-like organisms), which has been yet  
29 poorly investigated. Like the *Chlamydiaceae*, these *Chlamydia*-related bacteria are obligate  
30 intracellular bacteria that also exhibit a biphasic developmental cycle. Serological and  
31 molecular studies have implicated some species in various human and animal infections.  
32 *Parachlamydia acanthamoebae* is associated with human pneumonia (6, 12, 26, 27) and  
33 might cause bovine abortions (5, 38, 39), *Simkania negevensis* is responsible of respiratory  
34 infections, especially in children (18, 20, 22, 28, 32-35) whereas *Waddlia chondrophila* has  
35 been reported to cause abortion in bovines (14, 40) and is strongly suspected as an agent of  
36 miscarriage in human (3, 4). Some of these newly discovered *Chlamydia*-related bacteria  
37 that resist digestion by several environmental amoebae are also resistant to professional  
38 phagocytes of the innate immune system such as macrophages. Considering their potential  
39 threat on human health, it is important to be able to detect these obligate intracellular  
40 bacteria, since classical culture methods are ineffective. Thus, quantitative real-time PCRs  
41 have been developed (6, 21, 26, 31, 42), however they target specifically only one single  
42 species. Moreover, the only “broad-range” quantitative real-time PCR previously developed

43 in the field is a family-specific PCR amplifying DNA from members of the *Chlamydiaceae*  
44 family, which will not allow detection of *Chlamydia*-related bacteria (17). Since the  
45 biodiversity of *Chlamydiales* appears to be much larger than previously expected and new  
46 chlamydial strains are constantly discovered (7-9, 29, 30, 41), a molecular diagnostic tool  
47 able to detect any member of the *Chlamydiales* order is needed. Such a molecular tool would  
48 help in identifying the potential pathogenic role of *Chlamydia*-related bacteria and in  
49 specifying the true diversity of *Chlamydiales*, which is likely yet underestimated.  
50 Thus, we developed a *Chlamydiales*-specific real-time Taqman PCR (hereafter named pan-  
51 *Chlamydiales* PCR), that we validated using 128 clinical samples available from previous  
52 studies. We also applied this new PCR to 422 nasopharyngeal swabs samples taken from  
53 children with and without pneumonia, to investigate for the presence of chlamydial DNA.

54

## 55 MATERIAL AND METHODS

56 **DNA extraction.** Nasopharyngeal swabs samples were extracted automatically with the LC  
57 automated system (Roche, Rotkreuz, Switzerland) and the MagNA Pure LC DNA isolation kit  
58 I (Roche). Extracted DNAs were re-suspended in 100 µl of the provided elution buffer. One  
59 negative extraction control was included for each extraction run (32 wells/extraction run).

60 **Primers and probe.** Based on an alignment of the 16S ribosomal RNA sequences available  
61 in Genbank database (<http://www.ncbi.nlm.nih.gov/genbank/>), specific primers and probe  
62 were designed using the Geneious software 5.0.3 and primer3Plus (37). Locked Nucleic  
63 Acids (underlined below) were added to ensure a higher specificity. We chose a primer  
64 forward panCh16F2 (5'-CCGCCAACACTGGGACT-3'), a primer reverse panCh16R2 (5'-  
65 GGAGTTAGCCGGTGCTTCTTTAC-3') and a probe panCh16S (5'-FAM [6-carboxyfluorescein]-

66 CTACGGGAGGCTGCAGTCGAATC-BHQ1 [Black Hole Quencher]-3'), targeting a fragment  
67 of about 207 to 215 bp in the 16S ribosomal RNA gene (length variable according to the  
68 species).

69 **Real-time PCR assay.** PCR assays were performed in 20 µl, with iTaq supermix with ROX  
70 (BioRad, Reinach, Switzerland), 0.1 µM of each primer (Eurogentec, Seraing, Belgium), 0.1  
71 µM of probe (Eurogentec), molecular biology grade water (Sigma-Aldrich, Buchs,  
72 Switzerland) and 5 µl of DNA sample. Cycling conditions were 3 min at 95°C, followed by 50  
73 3-steps cycles of 15 s at 95°C, 15 s at 67°C and 15 s at 72°C. PCR products, tested in  
74 duplicate, were detected with a StepOne instrument (Applied Biosystems, Zug, Switzerland)  
75 for children nasopharyngeal swabs and with a ABI 7900 (Applied Biosystems) for analytic  
76 validation on samples from the retrospective study. Water was used as a negative PCR  
77 control.

78 **Quantification and positive recombinant plasmid control.** DNA from *Parachlamydia*  
79 *acanthamoebae* strain Hall's coccus was isolated from a purified bacterial culture available  
80 in our laboratory, using the Wizard Genomic DNA purification kit (Promega, Duebendorf,  
81 Switzerland). A PCR reaction was performed using the polymerase AmpliTaq Gold (Applied  
82 Biosystems) and the primers Pacstd16SF2 (5'-GCTGACGGCGTGGATGAGGC-3') and  
83 Pacstd16SR2 (5'-CCTACGCGCCCTTTACGCCC-3'). The PCR products were purified with the  
84 MSB Spin PCRapace kit (Invitex, Berlin, Germany) and cloned according to the  
85 manufacturer's protocol, in the pCR2.1-TOPO vector (Invitrogen, Basel, Switzerland)  
86 containing ampicillin and tetracycline resistance genes. Isolation of plasmidic DNA was  
87 performed with the QIAprep Spin Miniprep Kit (Qiagen, Kombrechtikon, Switzerland). The  
88 construction was checked by sequencing, using primers of the pCR2.1-TOPO vector

89 provided in the kit. Quantification of the recombinant plasmid was done on a Nanodrop ND-  
90 1000 (Witech, Littau, Switzerland), and serial dilutions ( $10^5$  to  $10^0$  copies/ $\mu$ l) were used as  
91 positive controls, to establish a standard curve for quantification and to check the  
92 reproducibility and efficiency of detection (see below). Negative controls, standard curve  
93 and samples were all analyzed in duplicate.

#### 94 **Analytical specificity, efficiency and reproducibility of the PCR**

95 The specificity of the new quantitative PCR was tested using DNA extracted from different  
96 bacteria commonly found in respiratory tract samples (Table 1). DNAs were diluted at  $10^5$   
97 copies of the 16S rRNA gene per reaction. Using the positive control plasmid, the analytical  
98 sensitivity and the reproducibility of the PCR was assessed on duplicates with 10-fold  
99 dilutions ( $5 \times 10^5$  to  $5 \times 10^0$  copies/reaction) in 12 independent runs. The efficiency of  
100 detection was performed with the positive control plasmid diluted at 50, 20, 5, 1 and 0.5  
101 DNA copies per reaction; each concentration tested in 20 replicates. The range of the PCR  
102 was also evaluated with chlamydial DNA from 15 different strains (Table 2).

103 **Clinical samples.** The new pan-*Chlamydiales* PCR was validated on 128 clinical samples.  
104 Different clinical samples including urines, cervico-vaginal, anorectal and nasopharyngeal  
105 swabs were collected and DNA was extracted between 2004 and 2010 by the diagnostic  
106 laboratory of the Institute of Microbiology, Lausanne, Switzerland (Table 3). These samples  
107 were originally tested with a real-time PCR specific of *Chlamydia trachomatis* (113 samples)  
108 (2, 13) and with a multiplex real-time PCR (42) detecting specifically *Chlamydia*  
109 *pneumoniae* but also *Mycoplasma pneumoniae* and *Legionella pneumophila* (15 samples).  
110 Positive samples for *M. pneumoniae* (5 samples) or *L. pneumophila* (3 samples) were  
111 included to confirm the high specificity of the new real-time PCR. We then applied our new

112 pan-*Chlamydiales* PCR to 422 nasopharyngeal swabs prospectively collected between 2008  
113 and 2010 at the University Hospitals of Geneva from children with (n=265) or without  
114 (n=157) pneumonia. Pneumonia was defined by the presence of at least one of the  
115 following symptoms: fever (>38°C), cough, dyspnea, tachypnea and an infiltrate or a  
116 consolidation at the lung X-ray. All samples were systematically tested for the following  
117 viruses by PCR: respiratory syncytial virus A, B, adenovirus A, B, C and E, coronavirus  
118 HKU1, OC43, 229E, NL63, parainfluenzae virus 1, 2 and 3, HMPV A, B, enterovirus A, B, C, D,  
119 rhinovirus A, B, influenza virus A, B and H1N1 for some samples during the 2009 epidemics.  
120 In addition, the nasopharyngeal samples were tested by PCR for the presence of  
121 *Streptococcus pneumoniae* and by real-time PCR for *Mycoplasma pneumoniae* and *Legionella*  
122 *pneumophila*. Children were aged between 1 and 15 years old: median age in the group of  
123 pneumonia was 4.6 years old and 6.2 years old for the control group. All DNA samples were  
124 tested in duplicate. Positive samples were systematically confirmed in a second run. To test  
125 for potential false negative results due to PCR inhibitors, an inhibition test was  
126 systematically performed with 4 µl of clinical DNA samples and 1 µl of the positive control  
127 at a concentration of 200 DNA copies/µl. The PCR was considered inhibited when the  
128 quantification was below 50 DNA copies per reaction (four-fold reduction). Moreover, a  
129 total of 60 non inoculated swabs (Copan, Brescia, Italy) were used as an additional negative  
130 control, to check that the commercial swabs used in the prospective study were not  
131 contaminated with any chlamydial DNA.

132 **Sequencing of positive samples.** Amplicons of positive samples were purified using the  
133 MSB Spin PCRapace kit (Invitex). A sequencing PCR was performed with specifically  
134 designed inner primers panFseq (5'-CCAACACTGGGACTGAGA-3') and panRseq (5'-



135 GCCGGTGCTTCTTTAC-3'). The sequencing PCR assay was done using the BigDye®  
136 Terminator v 1.1 Cycle seq kit (Applied Biosystems). Sequences of positive nasopharyngeal  
137 samples taken from children have been deposited on the NCBI website. Accession numbers  
138 are HQ721193 to HQ721240.

139

## 140 RESULTS

### 141 **Sensitivity and specificity of the pan-*Chlamydiales* quantitative PCR**

142 No cross-reaction was observed with the different bacterial or amoebal strains tested  
143 (Table 1). A competition test was also performed by testing an increasing amount of DNA  
144 from *Protochlamydia naegleriophila* strain KNic (from 0 to 10<sup>3</sup> copies of the 16S rRNA gene  
145 per reaction) in the presence of an increasing amount of a mixture of non chlamydial DNA  
146 (Table 1) (from 0 to 10<sup>6</sup> copies of the 16S rRNA gene per reaction). The amplification of the  
147 DNA from *P. naegleriophila* strain KNic was not affected by competing non chlamydial DNA  
148 up to 10<sup>5</sup> copies of the 16S rRNA gene of non targeted bacteria, demonstrating the high  
149 specificity of the PCR. The range of the new PCR was evaluated with 15 DNAs from different  
150 chlamydial strains (Table 2). As expected, all the different members of the *Chlamydiales*  
151 order tested were detected, confirming the large range of the PCR. Despite the presence of 1  
152 mismatch with the probe in the 16S rDNA sequence of *C. psittaci* and *C. abortus*, both  
153 species were successfully amplified. Alignment of all other sequences available from  
154 members of the Chlamydiales order demonstrated that 1 mismatch is also present for *C.*  
155 *caviae*, *C. felis*, and Candidatus *Clavochlamydia salmonicola* in the probe or for  
156 *Rhabdochlamydia porcellionis* and *R. crassificans* in the forward primer. These species are  
157 nevertheless likely all amplified with our new pan-*Chlamydiales* PCR. Indeed, numerous

158 DNAs somehow related to *Rhabdochlamydiaceae* have been successfully amplified from  
159 clinical samples (see below). The only known member of the *Chlamydiales* order likely not  
160 amplified using our pan-*Chlamydiales* PCR is *Piscichlamydia salmonis*, since as many as 6  
161 mismatches are present

### 162 **Reproducibility and efficiency of the pan-*Chlamydiales* real-time PCR**

163 The inter-run and intra-run reproducibility was assessed respectively on 12 independent  
164 runs and 72 duplicates, which results are shown in Figure 1 (A and B). All duplicates were  
165 amplified for 50 and more DNA copies per reaction and 18 replicates out of 24 (75%) for 5  
166 DNA copies per reaction. The Bland-Altman graph clearly indicates that differences  
167 between duplicates were below 1 cycle threshold (Ct) for DNA copies above 50 per  
168 reaction, demonstrating a high reproducibility. The efficiency of detection was evaluated on  
169 20 replicates for 50, 20, 5, 1 and 0.5 DNA copies per reaction. The PCR showed 100%  
170 detection for 50 and 20 DNA copies, 75%, 30% and 5% for 5, 1 and 0.5 DNA copies per  
171 reaction respectively (Fig. 1C).

### 172 **Analytical validation of the new PCR**

173 Over the 65 samples positive for *Chlamydia trachomatis* or *C. pneumoniae*, 61 (93.8%)  
174 samples were found positive with the new PCR (Table 3A and B). The 4 discordant samples  
175 were originally positive for *C. trachomatis*, from anorectal swabs (n=2), urine (n=1) and  
176 ascitis liquid (n=1). These 4 samples were tested a second time with the original test (*C.*  
177 *trachomatis* real-time PCR) and were found negative (n=1) or positive with only 0.2, 6 and  
178 1.2 copies per reaction, which was most certainly below the detection limits of the pan-  
179 *Chlamydiales* PCR. Seven positive samples with the pan-*Chlamydiales* PCR (cycle threshold  
180 values from 23.6 to 41.3) were sequenced to confirm the results. All the sequences obtained

181 showed 100% similarity with the expected species (Supplementary table S1), confirming  
182 the specificity of the new PCR and the possible identification by sequencing even with later  
183 cycle threshold values. Positive samples for *Mycoplasma pneumoniae* (n=5) and *Legionella*  
184 *pneumophila* (n=3) were all found negative with the new PCR (Table 3A). On the total of 63  
185 samples negative for *C. trachomatis* or *C. pneumoniae*, only 1 sample was amplified, showing  
186 92% with the closest previously described *Protochlamydia naegleriophila* strain CRIB 41  
187 (FJ532294.1) (Table 3B).

### 188 **Application of the quantitative PCR**

189 The application of the new pan-*Chlamydiales* PCR was on 422 nasopharyngeal swabs  
190 samples taken from children revealed 48 positive samples: 31 (7.3%) samples with 1/4  
191 positive wells, 6 (1.4%) samples with 2/4 positive wells, 4 (0.9%) samples with 3/4  
192 positive wells and 7 (1.7%) samples with 4/4 positive wells (Supplementary Table S2). A  
193 correlation between the cycle threshold value (Ct) and the number of positive wells was  
194 observed (Supplementary figure S1). Samples with <5 DNA copies per reaction (high Ct  
195 values) were amplified in 3/4, 2/4 and 1/4 wells. The 48 positive samples were sequenced  
196 and 48 sequences were obtained from 45 different patients (Supplementary Table S2).  
197 Indeed, the sequencing of 3 samples failed and for 3 others samples, 2 different sequences  
198 were obtained (Patients GE10169, HE210023, HE210045, see Table S2). Thus 94% of the  
199 positive samples were successfully sequenced. Patients' characteristics and sequencing  
200 results for patients with pneumonia are presented in Table 4. Among these 25 patients  
201 listed in Table 4, another etiology was identified for only 8 patients.

202 A percentage of similarity for the best BLAST greater than 90% was observed for all the 48  
203 sequences obtained, allowing identification at least at the family level. On the 48 sequences

204 obtained, 26 belonged to the *Parachlamydiaceae* family, 7 to the *Chlamydiaceae* family, 5 to  
205 the *Simkaniaceae* family, 5 to the *Criblamydiaceae* family, 3 to the *Rhabdochlamydiaceae*  
206 family, 1 seemed to belong to the novel E6-lineage (7, 11) and 1 other sequence  
207 corresponded to an unclassified *Chlamydiales* (Table S2). Among the 7 sequences  
208 corresponding to a *Chlamydiaceae* species, 6 showed 100% similarity with *Chlamydia*  
209 *pneumoniae*: 5 samples were taken from children with pneumonia (Table 4) whereas 1 was  
210 taken from an apparently healthy child (Supplementary Table S2). This latter patient had a  
211 previous history of obstructive bronchitis and chronic otitis media. The remaining  
212 *Chlamydiaceae* sequence showed 100% similarity with *C. trachomatis* (the sample was  
213 taken from a child with pneumonia) (Table 4). Among the 26 sequences corresponding to a  
214 member of the *Parachlamydiaceae* family, 10 (40%) were taken from 10 patients with  
215 pneumonia and 16 (60%) from 15 patients from the control group (patient HE210023  
216 being positive for 2 different bacteria). These latter patients were positive in 4/4, 3/4, 2/4  
217 and 1/4 positive wells, respectively for 2, 2, 3 and 18 nasopharyngeal swabs (Table S2).  
218 *Criblamydiaceae* species were recovered from 4 patients with pneumonia (all with 1/4  
219 positive well) and 1 patient from the control group (4/4 positive wells). *Simkaniaceae*  
220 species were found in 5 patients (3 control patients and 2 children with pneumonia).  
221 Finally, *Rhabdochlamydiaceae* species were identified in 1 case of pneumonia and 2 control  
222 subjects. Thus, 17 and 20 children with and without pneumonia respectively, were positive  
223 for a *Chlamydia*-related bacterium. In addition, a sample taken from a control subject could  
224 not be affiliated in any range of family-level lineage (unclassified *Chlamydiales*).

225 All 60 non inoculated Copan swabs were found negative with the pan-*Chlamydiales* PCR,  
226 demonstrating that the positive samples were not false positive. Furthermore, no absence

227 of the internal amplification control was observed, excluding false negative results due to  
228 PCR inhibitors.

229

## 230 DISCUSSION

231 In this work, we developed a new *Chlamydiales*-specific PCR that proves to be specific to the  
232 *Chlamydiales* order, to be sensitive for at least 5 DNA copies per reaction of the positive  
233 control (with an efficiency of 75%) and to be highly reproducible. Moreover, its application  
234 to clinical samples taken from children with and without pneumonia demonstrated the  
235 common exposure of humans to various *Chlamydia*-related bacteria. This new PCR showed  
236 a broad range of targeted species since it detected the 15 different chlamydial strains tested  
237 and the DNAs of 36 never described species-level lineages (<97% similarity of the 16S  
238 rDNA sequence) of the *Chlamydiales* order (>80% similarity of the 16S rDNA sequence)  
239 (16, 25) present in nasopharyngeal swabs samples (Supplementary Table S2). Furthermore,  
240 this new PCR could detect chlamydial DNA from samples of various origins (Table 3).

241 Previous classical pan-*Chlamydiales* PCRs have already been developed (10, 36, 43) but they  
242 detected from 1000 DNA copies compared to real-time PCRs that can detect about 200 to  
243 1000-fold less DNA copies per reaction. This higher sensitivity is likely due to the shorter  
244 reads (about 200 bp) and the read-out thank to a fluorescent Taqman probe. Considering  
245 this high sensitivity, DNA extraction, real-time PCR and sequencing reactions were  
246 processed in separate rooms to avoid contaminations between samples. In addition,  
247 automated DNA extraction located outside from our research laboratory was preferred.  
248 Moreover, since no sequence obtained showed more than 97% similarity with bacteria  
249 grown in our laboratory, a contamination may not explain the obtained results. The

250 sequencing of most positive samples was possible and results were informative at the  
251 family-level. A previous study using short sequences of *Chlamydiales* also successfully  
252 identified strains at the family-level with similar length sequences (140 to 195 bp) (43).  
253 Further identification, at the species-level, may be performed using complementary  
254 methods (PCR targeting a more discriminative core gene such as *rpoB* or *gyrA*).

255 As previous studies on nasal and/or nasopharyngeal samples have already allowed the  
256 recovery of *Chlamydia*-related bacteria or the amplification of DNA of these obligate  
257 intracellular bacteria (1, 12, 15, 36), we chose similar samples for the first application of the  
258 new PCR. The sequencing results on these nasopharyngeal swabs confirmed previous  
259 studies on the occurrence of *Chlamydia*-related bacteria in nasal mucosa of healthy  
260 individuals (1). They also clearly showed that the biodiversity of *Chlamydia*-related bacteria  
261 is far from being established: among the 48 sequences, 36 were from putative new species,  
262 when considering the Everett cut-off of < 97% 16S rRNA similarity to define species-level  
263 lineages and all were belonging to the *Chlamydiales* order (>80% similarity of the 16S rDNA  
264 sequence) (16, 23, 24). Thus, our work clearly demonstrates the common exposure of  
265 children to different *Chlamydiales*, since around 11.4% of patients were positive with the  
266 new PCR. When a *Chlamydiaceae* species was amplified, it was generally from a sample  
267 taken from a child with pneumonia (6/7). Noteworthy, DNA of *Criblamydiaceae* were also  
268 mainly amplified from patients with pneumonia (4/5), whereas other *Chlamydia*-related  
269 bacteria were amplified from nasopharyngeal swabs taken from both children with and  
270 without pneumonia. Thus, although our study demonstrated a common exposure to  
271 *Parachlamydiaceae*, (amplified from 5.9% of all samples), these were not over-expressed in  
272 the pneumonia group. Nonetheless, since the sequencing does not allow identification at

273 the species level, a significant correlation with a given species may not be excluded.  
274 Similarly, our work did not bring any argument in favor of an association of *Simkaniaceae*  
275 with pneumonia in children. This was somehow expected, since initial studies that  
276 suggested an association of *Simkania negevensis* with diverse respiratory infections in  
277 children (15, 18-20, 22, 32, 33, 35) were not confirmed in more recent works (34). Further  
278 research is now needed to specify the pathogenic role of each representing species in the  
279 *Chlamydiales* order.

280 In conclusion, this work provides a new diagnostic approach to specify the biodiversity and  
281 pathogenic role of *Chlamydia*-related bacteria and highlights the common exposure of  
282 children to *Parachlamydiaceae*.

283

284 **Acknowledgments**

285 J. Lienard is working at the Center for Research on Intracellular Bacteria (CRIB) thank to  
286 financial support from SUEZ-Environment (CIRSEE). G. Greub is supported by the Leenards  
287 Foundation through a career award entitled 'Bourse Leenards pour la relève académique en  
288 médecine clinique à Lausanne'.

289 We thank René Brouillet for technical help.



## 291 REFERENCES

- 292 1. **Amann, R., N. Springer, W. Schonhuber, W. Ludwig, E. N. Schmid, K. D. Muller,**  
293 **and R. Michel.** 1997. Obligate intracellular bacterial parasites of acanthamoebae related  
294 to *Chlamydia* spp. Appl Environ Microbiol **63**:115-21.
- 295 2. **Baud, D., K. Jaton, C. Bertelli, J. P. Kulling, and G. Greub.** 2008. Low prevalence of  
296 *Chlamydia trachomatis* infection in asymptomatic young Swiss men. BMC Infect Dis  
297 **8**:45.
- 298 3. **Baud, D., L. Regan, and G. Greub.** 2008. Emerging role of *Chlamydia* and *Chlamydia*-  
299 like organisms in adverse pregnancy outcomes. Curr Opin Infect Dis **21**:70-6.
- 300 4. **Baud, D., V. Thomas, A. Arafa, L. Regan, and G. Greub.** 2007. *Waddlia*  
301 *chondrophila*, a potential agent of human fetal death. Emerg Infect Dis **13**:1239-43.
- 302 5. **Borel, N., S. Ruhl, N. Casson, C. Kaiser, A. Pospischil, and G. Greub.** 2007.  
303 *Parachlamydia* spp. and related *Chlamydia*-like organisms and bovine abortion. Emerg  
304 Infect Dis **13**:1904-7.
- 305 6. **Casson, N., K. M. Posfay-Barbe, A. Gervaix, and G. Greub.** 2008. New diagnostic  
306 real-time PCR for specific detection of *Parachlamydia acanthamoebae* DNA in clinical  
307 samples. J Clin Microbiol **46**:1491-3.
- 308 7. **Corsaro, D., V. Feroldi, G. Saucedo, F. Ribas, J. F. Loret, and G. Greub.** 2009. Novel  
309 *Chlamydiales* strains isolated from a water treatment plant. Environ Microbiol **11**:188-  
310 200.
- 311 8. **Corsaro, D., R. Michel, J. Walochnik, K. D. Muller, and G. Greub.** 2010.  
312 *Saccamoeba lacustris*, sp. nov. (*Amoebozoa: Lobosea: Hartmannellidae*), a new lobose  
313 amoeba, parasitized by the novel chlamydia 'Candidatus *Metachlamydia lacustris*'  
314 (*Chlamydiae: Parachlamydiaceae*). Eur J Protistol **46**:86-95.
- 315 9. **Corsaro, D., and D. Venditti.** 2009. Detection of *Chlamydiae* from freshwater  
316 environments by PCR, amoeba coculture and mixed coculture. Res Microbiol **160**:547-  
317 52.
- 318 10. **Corsaro, D., D. Venditti, A. Le Faou, P. Guglielmetti, and M. Valassina.** 2001. A new  
319 chlamydia-like 16S rDNA sequence from a clinical sample. Microbiology **147**:515-6.
- 320 11. **Corsaro, D., D. Venditti, and M. Valassina.** 2002. New chlamydial lineages from  
321 freshwater samples. Microbiology **148**:343-4.
- 322 12. **Corsaro, D., D. Venditti, and M. Valassina.** 2002. New parachlamydial 16S rDNA  
323 phlotypes detected in human clinical samples. Res Microbiol **153**:563-7.

- 324 13. **Dang, T., K. Jatton-Ogay, M. Flepp, H. Kovari, J. M. Evison, J. Fehr, P. Schmid, E.**  
325 **Boffi El Amari, M. Cavassini, M. Odorico, P. E. Tarr, and G. Greub.** 2009. High  
326 prevalence of anorectal chlamydial infection in HIV-infected men who have sex with men  
327 in Switzerland. *Clin Infect Dis* **49**:1532-5.
- 328 14. **Dilbeck-Robertson, P., M. M. McAllister, D. Bradway, and J. F. Evermann.** 2003.  
329 Results of a new serologic test suggest an association of *Waddlia chondrophila* with  
330 bovine abortion. *J Vet Diagn Invest* **15**:568-9.
- 331 15. **Don, M., M. Paldanius, L. Fasoli, M. Canciani, and M. Korppi.** 2006. *Simkania*  
332 *negevensis* and pneumonia in children. *Pediatr Infect Dis J* **25**:470-1; author reply 471-2.
- 333 16. **Everett, K. D., R. M. Bush, and A. A. Andersen.** 1999. Emended description of the  
334 order *Chlamydiales*, proposal of *Parachlamydiaceae* fam. nov. and *Simkaniaceae* fam.  
335 nov., each containing one monotypic genus, revised taxonomy of the family  
336 *Chlamydiaceae*, including a new genus and five new species, and standards for the  
337 identification of organisms. *Int J Syst Bacteriol* **49 Pt 2**:415-40.
- 338 17. **Everett, K. D., L. J. Hornung, and A. A. Andersen.** 1999. Rapid detection of the  
339 *Chlamydiaceae* and other families in the order *Chlamydiales*: three PCR tests. *J Clin*  
340 *Microbiol* **37**:575-80.
- 341 18. **Fasoli, L., M. Paldanius, M. Don, F. Valent, L. Vetrugno, M. Korppi, and M.**  
342 **Canciani.** 2008. *Simkania negevensis* in community-acquired pneumonia in Italian  
343 children. *Scand J Infect Dis* **40**:269-72.
- 344 19. **Friedman, M. G., A. Galil, S. Greenberg, and S. Kahane.** 1999. Seroprevalence of IgG  
345 antibodies to the chlamydia-like microorganism '*Simkania Z*' by ELISA. *Epidemiol Infect*  
346 **122**:117-23.
- 347 20. **Friedman, M. G., S. Kahane, B. Dvoskin, and J. W. Hartley.** 2006. Detection of  
348 *Simkania negevensis* by culture, PCR, and serology in respiratory tract infection in  
349 Cornwall, UK. *J Clin Pathol* **59**:331-3.
- 350 21. **Goy, G., A. Croxatto, K. M. Posfay-Barbe, A. Gervaix, and G. Greub.** 2009.  
351 Development of a real-time PCR for the specific detection of *Waddlia chondrophila* in  
352 clinical samples. *Eur J Clin Microbiol Infect Dis* **28**:1483-6.
- 353 22. **Greenberg, D., A. Banerji, M. G. Friedman, C. H. Chiu, and S. Kahane.** 2003. High  
354 rate of *Simkania negevensis* among Canadian inuit infants hospitalized with lower  
355 respiratory tract infections. *Scand J Infect Dis* **35**:506-8.
- 356 23. **Greub, G.** 2010. International Committee on Systematics of Prokaryotes. Subcommittee  
357 on the taxonomy of the *Chlamydiae*: minutes of the closed meeting, 21 June 2010, Hof  
358 bei Salzburg, Austria. *Int J Syst Evol Microbiol* **60**:2694.

- 359 24. **Greub, G.** 2010. International Committee on Systematics of Prokaryotes. Subcommittee  
360 on the taxonomy of the *Chlamydiae*: minutes of the inaugural closed meeting, 21 March  
361 2009, Little Rock, AR, USA. *Int J Syst Evol Microbiol* **60**:2691-3.
- 362 25. **Greub, G.** 2009. *Parachlamydia acanthamoebae*, an emerging agent of pneumonia. *Clin*  
363 *Microbiol Infect* **15**:18-28.
- 364 26. **Greub, G., P. Berger, L. Papazian, and D. Raoult.** 2003. *Parachlamydiaceae* as rare  
365 agents of pneumonia. *Emerg Infect Dis* **9**:755-6.
- 366 27. **Greub, G., I. Boyadjiev, B. La Scola, D. Raoult, and C. Martin.** 2003. Serological hint  
367 suggesting that *Parachlamydiaceae* are agents of pneumonia in polytraumatized intensive  
368 care patients. *Ann N Y Acad Sci* **990**:311-9.
- 369 28. **Heiskanen-Kosma, T., M. Paldanius, and M. Korppi.** 2008. *Simkania negevensis* may  
370 be a true cause of community acquired pneumonia in children. *Scand J Infect Dis* **40**:127-  
371 30.
- 372 29. **Horn, M.** 2008. *Chlamydiae* as symbionts in eukaryotes. *Annu Rev Microbiol* **62**:113-31.
- 373 30. **Horn, M., and M. Wagner.** 2001. Evidence for additional genus-level diversity of  
374 *Chlamydiales* in the environment. *FEMS Microbiol Lett* **204**:71-4.
- 375 31. **Jaton, K., J. Bille, and G. Greub.** 2006. A novel real-time PCR to detect *Chlamydia*  
376 *trachomatis* in first-void urine or genital swabs. *J Med Microbiol* **55**:1667-74.
- 377 32. **Kahane, S., D. Greenberg, M. G. Friedman, H. Haikin, and R. Dagan.** 1998. High  
378 prevalence of "Simkania Z," a novel *Chlamydia*-like bacterium, in infants with acute  
379 bronchiolitis. *J Infect Dis* **177**:1425-9.
- 380 33. **Korppi, M., M. Paldanius, A. Hyvarinen, and A. Nevalainen.** 2006. *Simkania*  
381 *negevensis* and newly diagnosed asthma: a case-control study in 1- to 6-year-old children.  
382 *Respirology* **11**:80-3.
- 383 34. **Kumar, S., S. A. Kohlhoff, M. Gelling, P. M. Roblin, A. Kutlin, S. Kahane, M. G.**  
384 **Friedman, and M. R. Hammerschlag.** 2005. Infection with *Simkania negevensis* in  
385 Brooklyn, New York. *Pediatr Infect Dis J* **24**:989-92.
- 386 35. **Nascimento-Carvalho, C. M., M. R. Cardoso, M. Paldanius, A. Barral, C. A. Araujo-**  
387 **Neto, A. Saukkoriipi, R. Vainionpaa, M. Leinonen, and O. Ruuskanen.** 2009.  
388 *Simkania negevensis* infection among Brazilian children hospitalized with community-  
389 acquired pneumonia. *J Infect* **58**:250-3.
- 390 36. **Ossewaarde, J. M., and A. Meijer.** 1999. Molecular evidence for the existence of  
391 additional members of the order Chlamydiales. *Microbiology* **145 ( Pt 2)**:411-7.
- 392 37. **Rozen, S., and H. Skaletsky.** 2000. Primer3 on the WWW for general users and for  
393 biologist programmers. *Methods Mol Biol* **132**:365-86.

- 394 38. **Ruhl, S., N. Casson, C. Kaiser, R. Thoma, A. Pospischil, G. Greub, and N. Borel.**  
395 2009. Evidence for *Parachlamydia* in bovine abortion. *Vet Microbiol* **135**:169-74.
- 396 39. **Ruhl, S., G. Goy, N. Casson, R. Thoma, A. Pospischil, G. Greub, and N. Borel.** 2008.  
397 *Parachlamydia acanthamoebae* infection and abortion in small ruminants. *Emerg Infect*  
398 *Dis* **14**:1966-8.
- 399 40. **Rurangirwa, F. R., P. M. Dilbeck, T. B. Crawford, T. C. McGuire, and T. F.**  
400 **McElwain.** 1999. Analysis of the 16S rRNA gene of micro-organism WSU 86-1044 from  
401 an aborted bovine foetus reveals that it is a member of the order *Chlamydiales*: proposal  
402 of *Waddliaceae* fam. nov., *Waddlia chondrophila* gen. nov., sp. nov. *Int J Syst Bacteriol*  
403 **49**:577-581.
- 404 41. **Thomas, V., N. Casson, and G. Greub.** 2006. *Criblamydia sequanensis*, a new  
405 intracellular *Chlamydiales* isolated from Seine river water using amoebal co-culture.  
406 *Environ Microbiol* **8**:2125-35.
- 407 42. **Welti, M., K. Jatton, M. Altwegg, R. Sahli, A. Wenger, and J. Bille.** 2003.  
408 Development of a multiplex real-time quantitative PCR assay to detect *Chlamydia*  
409 *pneumoniae*, *Legionella pneumophila* and *Mycoplasma pneumoniae* in respiratory tract  
410 secretions. *Diagn Microbiol Infect Dis* **45**:85-95.
- 411 43. **Wheelhouse, N., F. Katzer, F. Wright, and D. Longbottom.** 2010. Novel chlamydia-  
412 like organisms as cause of bovine abortions, UK. *Emerg Infect Dis* **16**:1323-4.
- 413
- 414

415  
416 Figure 1: Reproducibility and efficiency of the new real-time PCR. Inter and intra-run  
417 reproducibility was performed between 12 different runs representing 72 duplicates of  
418 positive control. (A) Inter-run variability. (B) Bland-Altman graph represents the intra-run  
419 variability between duplicates and a bias of 0.36 was calculating as well as the 95% limit of  
420 agreement shown by the dashed line. (C) Efficiency was evaluated with 20 replicates of 5  
421 different plasmid control concentration (50, 20, 5, 1 and 0.5 copies per reaction).

422 Supplementary figure S1: the graph shows cycle threshold (Ct) values according to the  
423 percentage of positive wells obtained for nasopharyngeal samples. The dashed line  
424 represents the mean Ct (36.3) obtained for 24 replicates of 5 DNA copies of the positive  
425 plasmid control per reaction (Fig.1A). The majority of clinical samples were detected at Ct  
426 values >36.3, corresponding to <5 DNA copies per reaction, for which the efficiency of the  
427 PCR decreases.

429 Table 1: Bacterial and amoebal species used to test the specificity.

BACTERIAL SPECIES	Source/strain
<i>Bacteroides fragilis</i> *	ATCC25825
<i>Escherichia coli</i> *	ATCC 25922
<i>Haemophilus influenzae</i> *	ATCC 49247
<i>Legionella pneumophila</i>	Clinical specimen
<i>Mycoplasma pneumoniae</i>	Clinical specimen
<i>Pseudomonas aeruginosa</i> *	ATCC 27853
<i>Staphylococcus aureus</i> *	ATCC 25923
<i>Streptococcus mitis</i>	ATCC 6249
<i>Streptococcus pneumoniae</i> *	Clinical specimen
AMOEBAL SPECIES	Source/strain
<i>Acanthamoeba castellanii</i>	ATCC 30010
<i>Acanthamoeba comandoni</i>	Strain WBT
<i>Dictyostelium discoideum</i>	DH1-10
<i>Hartmannella vermiformis</i>	ATCC 50237

430 \*Bacterial DNA used in the competition test with *Pr. naegleriophila* strain KNic.

431

432 Table 2: Chlamydial DNA used to evaluate the range of the new PCR

Chlamydial species	Source/strain
<i>Chlamydia abortus</i>	Strain S26/3 <sup>a</sup>
<i>Chlamydia pecorum</i>	Strain W73 <sup>b</sup>
<i>Chlamydia pneumoniae</i>	Strain K6 <sup>c</sup>
<i>Chlamydia psittaci</i>	Strain T49/90 <sup>d</sup>
<i>Chlamydia suis</i>	Strain S45/6 <sup>a</sup>
<i>Chlamydia trachomatis</i>	Clinical specimen
<i>Criblamydia sequanensis</i>	Strain CRIB-18
<i>Estrella lausannensis</i>	Strain CRIB-30
<i>Neochlamydia hartmannellae</i>	ATCC 50802
<i>Parachlamydia acanthamoebae</i>	Strain Hall's coccus
<i>Parachlamydia acanthamoebae</i>	ATCC VR-1476 (strain Bn9)
Candidatus <i>Protochlamydia amoebophila</i>	ATCC PRA-7 (strain UWE25)
<i>Protochlamydia naegleriophila</i>	Strain KNic
<i>Simkania negevensis</i>	ATCC VR-1471
<i>Waddlia chondrophila</i>	ATCC VR-1470

433 <sup>a</sup> Kindly provided by G.E. Jones, Moredun Research Institute, Edinburgh, UK

434 <sup>b</sup> Kindly provided by J. Storz, Baton Rouge Louisiana, LA, USA

435 <sup>c</sup> Kindly provided by A. Pospischil, Zürich, Switzerland

436 <sup>d</sup> Kindly provided by R.K. Hoop, Zürich, Switzerland

437

438 Table 3: Analysis of samples from various origins by the pan-*Chlamydiales* PCR in  
 439 comparison with the *C. pneumoniae* PCR (A) and the *C. trachomatis* PCR (B).

440 A

Samples	<i>C. pneumoniae</i>		Pan- <i>Chlamydiales</i>	
	+	-	+	-
Nasopharyngeal swabs	1	1 <sup>1/0</sup>	1	1
Bronchoalveolar lavages	0	6 <sup>2/1</sup>	0	6
Bronchial aspirates	0	4 <sup>0/2</sup>	0	4
Sputa	1	2 <sup>2/0</sup>	1	2
Sub-total	2	13	2	13
Total	15		15	

441 Superscript numbers indicate the number of positive sample for *Mycoplasma pneumoniae*  
 442 and the number of positive sample for *Legionella pneumophila* (*M.pn./L. pn.*), respectively

443 B

Samples	<i>C. trachomatis</i>		Pan- <i>Chlamydiales</i>	
	+	-	+	-
Vaginal or cervical swabs	14	15	14	15
Anorectal swabs	14	0	12	2**
Urethral swabs	1	0	1	0
Eye swabs	1	1	1	1
Urines	32	33	31(+1 <sup>°</sup> )	32(+1*)
Ascitis liquid	1	1	0	2*
Sub-total	63	50	60	53
Total	113		113	

444  
 445 \* 1 or \*\*2 sample(s) positive for *C. trachomatis* but negative with the pan-*Chlamydiales* PCR;  
 446 ° 1 sample negative for *C. trachomatis* but positive with the pan-*Chlamydiales* PCR.



447 Table 4: Sequencing results of nasopharyngeal samples from the pneumonia group positive with the new pan-*Chlamydiales*

448 PCR

Patient no.	Sex	Age (years)	Signs and symptoms	Other etiology	Underlying condition(s)	% 16S rRNA gene homology with most similar GenBank sequence (corresponding family)
GE10160	F	3.7	39.0°C, cough, thoracic pain, DRS	-	coeliakie	100% <i>Chlamydia pneumoniae</i> LPCoLN (Ch)
GE10097	F	2.7	40.6°C, cough, DRS	-	-	100% <i>Chlamydia pneumoniae</i> LPCoLN (Ch)
VS30014	M	12.4	38.9°C, cough	-	-	100% <i>Chlamydia pneumoniae</i> LPCoLN (Ch)
VS30030	F	12.2	39.5°C, cough	-	-	100% <i>Chlamydia trachomatis</i> D-LC (Ch)
GE10098	F	8.0	38.0°C, cough	-	-	100% <i>Chlamydia pneumoniae</i> CWL029 (Ch)
GE10014	M	7.6	39.5°C, cough	<i>M. pneumoniae</i>	-	94% Uncultured <i>Neochlamydia</i> sp. LTUNC09656 (P)
GE10159	M	3.7	40.0°C, cough	-	-	100% <i>Chlamydia pneumoniae</i> LPCoLN (Ch)
GE10169	M	5.6	40.0°C, cough, thoracic pain, tachypnea	-	Bronchodysplasia, premature birth (28 weeks)	97% Candidatus <i>Rhabdochlamydia porcellionis</i> (R) 91% <i>Chlamydiales</i> bacterium cvE38 (S)
GE10179	F	3.6	Dyspnea	<i>S. pneumoniae</i> H1N1 virus	-	Sequencing failed
HE20032	M	1.5	41.6°C, cough, DRS	-	-	94% Uncultured Candidatus <i>Protochlamydia</i> sp. clone CN823 (P)
VS30003	M	5.8	39.5°C, cough, DRS	-	-	95% Uncultured <i>Chlamydiales</i> bacterium clone P-5 (P)
GE10027	M	9.8	38.1°C, cough, DRS	<i>M. pneumoniae</i>	asthma	92% Uncultured soil bacterium clone 530-2 (Cr)
GE10036	M	1.6	38.0°C, cough, DRS, tachypnea	<i>S. pneumoniae</i>	-	95% Uncultured bacterium clone F5K2Q4C04JDDHX (P)
GE10047	M	2.6	39.5°C, cough, DRS, tachypnea	-	-	92% <i>Criblamydia sequanensis</i> (Cr)
GE10072	F	4.8	39.5 °C	HMPV A	-	Sequencing failed
GE10147	M	13.8	38.2°C, cough, DRS	<i>S. pneumoniae</i>	-	95% Uncultured bacterium clone FW1013-189 (P)

GE10193	F	5.1	38.9°C, cough, tachypnea	-	-	92% <i>Chlamydiales</i> bacterium cvE38 (S)
HE20008	F	3.3	38.3°C, cough, tachypnea, DRS	HUK1	-	93% <i>Estrella lausannensis</i> strain CRIB 30 (Cr)
HE20028	F	1.1	39.5°C, cough, DRS, tachypnea	HRSV A	-	94% Uncultured <i>Chlamydiales</i> bacterium clone P-5 (P)
HE20036	M	1.4	40.0°C, DRS	-	-	96% <i>Chlamydiales</i> bacterium cvE21 (E6)
HE20074	M	4.5	38.1°C, cough, DRS	-	-	94% <i>Criblamydia sequanensis</i> (Cr)
VS30007	M	6.6	38.7°C, cough, DRS	-	-	95% Candidatus <i>Metachlamydia lacustris</i> strain CHSL (P)
VS30013	M	6.4	38.5°C, cough, tachypnea	-	-	94% Uncultured <i>Chlamydiales</i> bacterium clone P-9 (P)
VS30044	M	3.8	40.4°C, cough	-	-	95% Uncultured <i>Chlamydiales</i> bacterium clone P-7 (P)
VS30055	F	4.1	38.5°C, cough, tachypnea	-	-	92% Candidatus <i>Metachlamydia lacustris</i> strain CHSL (P)

449 F= female, M = male; DRS = distress respiratory syndrome;

450 Ch= *Chlamydiaceae*, P = *Parachlamydiaceae*, R = *Rhabdochlamydiaceae*, S = *Simkaniaceae*, Cr = *Criblamydiaceae*, E6= novel E6-

451 lineage.


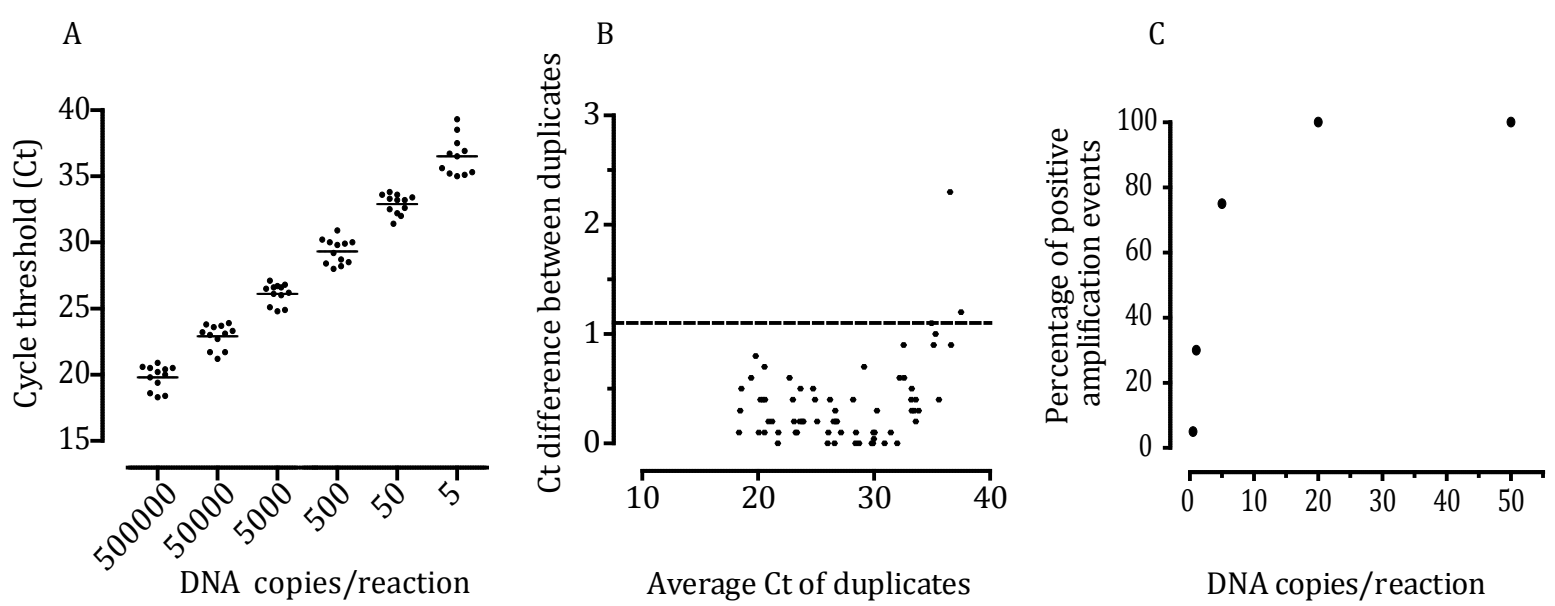


Figure 1: Reproducibility and efficiency of the new real-time PCR. Inter and intra-run reproducibility was performed between 12 different runs representing 72 duplicates of positive control. (A) Inter-run variability. (B) Bland-Altman graph represents the intra-run variability between duplicates and a bias of 0.36 was calculating as well as the 95% limit of agreement shown by the dashed line. (C) Efficiency was evaluated with 20 replicates of 5 different plasmid control concentration (50, 20, 5, 1 and 0.5 copies per reaction).

Table S1: Sequencing results of 7 samples from the retrospective study positive with the new PCR

Sample	Sequence (bp)	Threshold cycle (Ct) with the new PCR: mean $\pm$ SD	Expected result of the sequencing	% 16S rRNA gene sequence similarity with most similar GenBank sequence (Accession no.)
Sputa	183	36.1	CP +	100% <i>Chlamydia pneumoniae</i> LPCoLN (CP001713.1)
Nasopharyngeal swab	183	35.5 $\pm$ 0.7	CP +	100% <i>Chlamydia pneumoniae</i> LPCoLN (CP001713.1)
Cervical swab	192	23.6 $\pm$ 2.9	CT +	100% <i>Chlamydia trachomatis</i> D-LC (CP002054.1)
Anorectal swab	151	39.0 $\pm$ 0.2	CT +	100% <i>Chlamydia trachomatis</i> D-LC (CP002054.1)
Urine	192	35.0 $\pm$ 0.8	CT +	100% <i>Chlamydia trachomatis</i> D-LC (CP002054.1)
Cervical swab	206	29.3 $\pm$ 0.3	CT +	100% <i>Chlamydia trachomatis</i> D-LC (CP002054.1)
Urethral swab	141	31.7 $\pm$ 0.5	CT +	99% <i>Chlamydia trachomatis</i> D-LC (CP002054.1)
Urine	190	41.3	CT -	94% Uncultured bacterium clone FW1013-189 (EF693090.1)

CP = *Chlamydia pneumoniae*, CT = *C. trachomatis*.

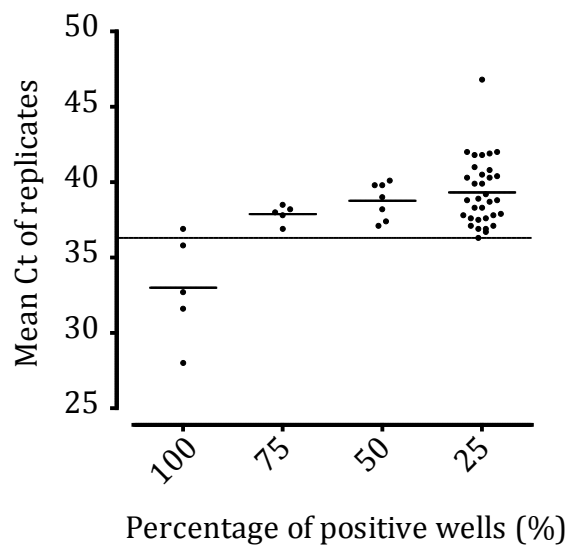

Supplementary figure S1: the graph shows cycle threshold (Ct) values according to the percentage of positive wells obtained for nasopharyngeal samples. The dashed line represents the mean Ct (36.3) obtained for 24 replicates of 5 DNA copies of the positive plasmid control per reaction (Fig.1A). The majority of clinical samples were detected at Ct values >36.3, corresponding to <5 DNA copies per reaction, for which the efficiency of the PCR decreases.