

Serveur Académique Lausannois SERVAL [serval.unil.ch](http://serval.unil.ch)

## Author Manuscript

Faculty of Biology and Medicine Publication

**This paper has been peer-reviewed but does not include the final publisher proof-corrections or journal pagination.**

Published in final edited form as:

**Title:** Derivation of new diagnostic reference levels for neuro-paediatric computed tomography examinations in Switzerland.

**Authors:** Wagner F, Bize J, Racine D, Le Coultre R, Verdun F, Trueb PR, Treier R

**Journal:** Journal of radiological protection : official journal of the Society for Radiological Protection

**Year:** 2018 Sep

**Issue:** 38

**Volume:** 3

**Pages:** 1013-1036

**DOI:** [10.1088/1361-6498/aac69c](https://doi.org/10.1088/1361-6498/aac69c)

In the absence of a copyright statement, users should assume that standard copyright protection applies, unless the article contains an explicit statement to the contrary. In case of doubt, contact the journal publisher to verify the copyright status of an article.



ACCEPTED MANUSCRIPT • OPEN ACCESS

## Derivation of new diagnostic reference levels for neuro-paediatric computed tomography examinations in Switzerland

To cite this article before publication: Franca Wagner *et al* 2018 *J. Radiol. Prot.* in press <https://doi.org/10.1088/1361-6498/aac69c>

### Manuscript version: Accepted Manuscript

Accepted Manuscript is “the version of the article accepted for publication including all changes made as a result of the peer review process, and which may also include the addition to the article by IOP Publishing of a header, an article ID, a cover sheet and/or an ‘Accepted Manuscript’ watermark, but excluding any other editing, typesetting or other changes made by IOP Publishing and/or its licensors”

This Accepted Manuscript is © 2018 IOP Publishing Ltd.

As the Version of Record of this article is going to be / has been published on a gold open access basis under a CC BY 3.0 licence, this Accepted Manuscript is available for reuse under a CC BY 3.0 licence immediately.

Everyone is permitted to use all or part of the original content in this article, provided that they adhere to all the terms of the licence <https://creativecommons.org/licenses/by/3.0>

Although reasonable endeavours have been taken to obtain all necessary permissions from third parties to include their copyrighted content within this article, their full citation and copyright line may not be present in this Accepted Manuscript version. Before using any content from this article, please refer to the Version of Record on IOPscience once published for full citation and copyright details, as permissions may be required. All third party content is fully copyright protected and is not published on a gold open access basis under a CC BY licence, unless that is specifically stated in the figure caption in the Version of Record.

View the [article online](#) for updates and enhancements.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

## Derivation of New Diagnostic Reference Levels for Neuro-Paediatric Computed Tomography Examinations in Switzerland

Franca Wagner,<sup>1</sup> Julie Bize,<sup>2</sup> Damien Racine,<sup>2</sup> Régis Le Coultre,<sup>3</sup> Francis Verdun<sup>2</sup>  
Philipp R. Trueb,<sup>4</sup> Reto Treier<sup>4</sup>

<sup>1</sup>Department of Diagnostic and Interventional Neuroradiology, University Hospital of Bern, University of Bern, Switzerland

<sup>2</sup>Institute of Radiation Physics, Lausanne University Hospital, Switzerland

<sup>3</sup>University of Health Sciences HESAV, HES-SO; University of Applied Sciences Western Switzerland, Lausanne, Switzerland

<sup>4</sup>Radiation Protection Division, Federal Office of Public Health, Bern, Switzerland

Corresponding author:

Franca Wagner, MD, Department of Diagnostic and Interventional Neuroradiology, University Hospital of Bern, University of Bern, Bern, Switzerland

Email: franca.wagner@insel.ch

Tel: 0041 31 632 26 54

Fax: 0041 31 632 48 72

**Manuscript type:** original article

**Word count:** 3493

**Running title:** New Diagnostic Reference Levels Neuro-Paediatric Switzerland

**Disclosure:** This study received no financial support.

**Abstract**

*Purpose:* Definition of new national diagnostic reference levels (DRLs) for volume computed tomography dose index (CTDI<sub>vol</sub>) and dose length product (DLP) for neuro-paediatric CT examinations depending on the medical indication.

*Methods:* Paediatric cranial CT data sets acquired between January 2013 and December 2016 were retrospectively collected between July 2016 and March 2017 from the eight largest university and cantonal hospitals that perform most of the neuro-paediatric CTs in Switzerland. A consensus review of CTDI<sub>vol</sub> and DLP was undertaken for the three defined anatomical regions: brain, facial bone and petrous bone; each with and without contrast medium application. All indications for cranial CT imaging in paediatrics were assigned to one of these three regions. Descriptive statistical analysis of the distribution of the median values for CTDI<sub>vol</sub> and DLP yielded minimum, maximum, 25th percentile (1st quartile), median (2nd quartile) and 75th percentile (3rd quartile). New DRLs for neuro-paediatric CT examinations in Switzerland were based on the 75th percentiles of the distributions of the median values of all eight centres. Where appropriate, values were rounded such that the DRLs increase or at least remain constant as the age of the patient increases.

*Results:* Our results revealed DRLs for CTDI<sub>vol</sub> and DLP up to 20% lower than the DRLs used so far in Switzerland and elsewhere in Europe.

*Conclusions:* This study provides Swiss neuro-paediatric CT DRL values to establish optimum conditions for paediatric cranial CT examinations. Periodic national updates of DRLs, following international comparisons, are essential.

## Article highlights

- A retrospective multicentre study enabled new national DRLs to be defined for volume computed tomography dose index (CTDI<sub>vol</sub>) and dose length product (DLP) of neuro-paediatric CT examinations in Switzerland.
- The strength, value, and originality of our method is that we propose new DRLs for medical indications.
- Data analysis of all neuro-paediatric CT scans resulted in DRLs up to 20% lower than those presently used in Switzerland and internationally for the three defined anatomical regions, brain, facial bone and petrous bone, specified according to the medical indication.
- The new DRLs are aimed to serve as an initial benchmark and guide the optimised application of CT protocols in neuroradiology departments in Swiss hospitals performing neuro-paediatric CT scans.

1  
2 **Keywords:** Radiation protection, radiation monitoring, CT, neuro-paediatrics, DRL,  
3  
4 CTDI<sub>vol</sub>, DLP  
5  
6

7 **Abbreviations:**  
8

9 CM contrast medium  
10  
11 CT computed tomography  
12  
13 CTDI<sub>vol</sub> volume computed tomography dose index  
14  
15  
16 DLP dose length product  
17  
18 DRL diagnostic reference level  
19  
20  
21 FOPH Federal Office of Public Health  
22  
23 MRI magnetic resonance imaging  
24  
25  
26 SL scan length  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

## 1. Introduction

Exposure of children to ionising radiation during computed tomography (CT) examinations is a cause for concern. Most neuro-paediatric CT examinations take place in emergency situations, and a 5-fold increase in frequency in the United States was documented from 1995 to 2008 [1]. This corresponds to a compound annual growth rate of 13.2% of paediatric emergency department visits that included a CT and a doubling time of approximately 5.6 years [1]. In 2008, CT was performed in 1.7 million of a total of 27.9 million paediatric visits to the emergency department [1]. Owing to its widespread availability, paediatric CT imaging is frequently used to enable correct diagnosis in the outpatient setting, e.g. for trauma and craniofacial surgery patients, who may undergo multiple head CTs during preoperative treatment and follow-up. Craniofacial paediatric CT imaging is commonly used for diagnostic evaluation, operative planning, and outcome analysis, despite increasing controversy regarding radiation exposure [2, 3]. The general increase of paediatric CT can be attributed to the availability of fast helical and multi-detector scanning, reducing the need for sedation and allowing the examination of younger, sicker and uncooperative children.

Many university and regional hospitals in Switzerland use low-dose CT protocols, which partly limit the diagnostic value in regard to the clinical indication and necessity of repetition [4]. Low-dose CT protocols reduce the amount of ionising radiation exposure for paediatric patients but image quality and diagnostic utility are often significantly compromised. Particularly in neurosurgical practice, children often require multiple brain CTs for some conditions e.g. hydrocephalus, intracranial haemorrhage, postoperative evaluation and intracranial infectious fluid collections. Neurosurgeons are looking for very specific information on the CT images, in terms

1  
2 of the pathology and anatomical position; a decreased image quality may not be  
3  
4 adequate. MRI – the imaging method of choice for children in most clinical  
5  
6 circumstances – is not available in every hospital at all times.  
7

8  
9 In 2012, Pearce et al. published a retrospective epidemiological study on the  
10  
11 relationship between paediatric head CTs and increased risk of developing brain  
12  
13 cancer and leukaemia. The authors reported that CT scans in children resulting in  
14  
15 cumulative doses of about 50 mGy, could almost triple the risk of leukaemia,  
16  
17 whereas doses of about 60 mGy might triple the risk of brain cancer [5]. Mathews et  
18  
19 al. reviewed a large cohort study of 680,000 children in Australia who underwent a  
20  
21 CT examination between 1985 and 2005; a 24% higher cancer incidence in exposed  
22  
23 than in non-exposed children was observed [6]. In 2013, the United Nations Scientific  
24  
25 Committee on the Effects of Atomic Radiation considered the effects of radiation  
26  
27 exposure on children and concluded that for a given radiation dose, children are  
28  
29 generally at more risk of tumour induction than adults [7]. This emphasises that the  
30  
31 estimates of lifetime cancer risk for those exposed as children might be a factor of 2  
32  
33 to 3 times higher than estimates for a population exposed at all ages [7].  
34  
35  
36  
37  
38

39 These studies, together with the ‘as low as reasonably achievable’ (ALARA)  
40  
41 concept in radiation protection, triggered worldwide awareness of the need for  
42  
43 justification of paediatric CT examinations and optimisation of doses [8]. This led the  
44  
45 International Commission on Radiological Protection (ICRP) to introduce the concept  
46  
47 of diagnostic reference levels (DRLs) [9]. The objective was to suggest radiation  
48  
49 dose levels for CTs under defined conditions in standard patients [10]. DRLs are not  
50  
51 dose limits for individual patient examinations, rather they are used to identify those  
52  
53 situations in which, for a specific radiological procedure, unusually high or low doses  
54  
55 necessitate optimisation actions [10–13]. In recent years, DRLs have proved to be a  
56  
57  
58  
59  
60



1  
2 valuable tool to reduce large differences in CT radiation doses between different  
3  
4 radiological facilities. However, since the DRL is defined as the 75th percentile of the  
5  
6 dose distribution, there is still a large potential to achieve further dose optimisation  
7  
8 [10].  
9

10  
11 Paediatric CTs in small- and medium-sized hospitals are obviously performed  
12  
13 much less often than adult CTs. The medical staff lack relevant experience and the  
14  
15 use of the paediatric CT protocols is not optimised [14–19]. It is important to pay  
16  
17 particular attention to paediatric CTs, because children are much more sensitive to  
18  
19 ionising radiation than adults [16, 17]. Reliable CT scanning in a safe and effective  
20  
21 manner is challenging in children because body size must be more carefully  
22  
23 considered, patient cooperation and understanding is often limited or absent, and  
24  
25 there is a lower tolerance for CT protocol errors in paediatrics [16, 17].  
26  
27  
28

29  
30 The purpose of our retrospective multicentre study was to define new national  
31  
32 DRLs for volume computed tomography dose index ( $CTDI_{vol}$ ) and dose length  
33  
34 product (DLP) of the most frequently performed neuro-paediatric CT examinations in  
35  
36 Switzerland. These new DRLs are aimed to serve as an initial benchmark and  
37  
38 provide guidance for the optimised application of CT protocols in neuroradiology  
39  
40 departments in Swiss hospitals performing paediatric CTs. The strength, value, and  
41  
42 originality of our study is that we propose DRLs for medical indications. The DRLs of  
43  
44 other European countries were used for comparison.  
45  
46  
47  
48  
49

## 50 **2. Materials and methods**

51  
52 According to the Swiss radiation protection legislation (Radiological Protection  
53  
54 Ordinance, Article 34, paragraph 2), the radiation protection authority is allowed to  
55  
56  
57  
58  
59  
60

1 collect and process anonymized data of radiological examinations and, for this  
2  
3  
4 reason, no ethical approval was required for this study.  
5  
6  
7

### 8 **Data collection**

9  
10 Paediatric cranial CT data sets acquired between January 2013 and December 2016  
11  
12 were retrospectively collected during a 9-month period (July 2016 to March 2017)  
13  
14 from the eight largest university and cantonal hospitals in Switzerland performing  
15  
16 most of the neuro-paediatric CTs nationwide. The participating hospitals were the  
17  
18 university hospitals of Geneva, Lausanne, Bern, Basel and Zurich and the cantonal  
19  
20 university hospitals of Geneva, Lausanne, Bern, Basel and Zurich and the cantonal  
21  
22 hospitals of Chur, Aarau and Lucerne.  
23

24 Anonymised dose data were collected from four Siemens CT scanners  
25  
26 (Somatom Definition Edge), four GE CT scanners (Brightspeed 8, Discovery 750 HD,  
27  
28 Lightspeed VCT, Revolution), three Toshiba CT scanners (Aquilion CXL, Aquilion  
29  
30 One, Aquilion RXL) and one Philips CT scanner (Brilliance CT 64). The cantonal  
31  
32 hospital of Aarau and the university hospital of Lausanne each provided dose data  
33  
34 from three CT scanners; the other hospitals provided dose data from one CT  
35  
36 scanner. In four hospitals, data were collected using commercial dose management  
37  
38 software; in two hospitals, data were collected using data collection software  
39  
40 developed in-house; and in two hospitals, data were manually registered in specific  
41  
42 spreadsheets. The collected dose data were summarised in an Excel spreadsheet  
43  
44 and sent to the project coordinator for analysis. Throughout the period of data  
45  
46 collection, the project coordinator maintained close contact with the participating  
47  
48 centres to provide support and clarification and give feedback when potential for  
49  
50 increased efficiency was seen.  
51  
52  
53  
54  
55  
56  
57

### 58 **2.1 Patient data**

1  
2 The study population of children aged from 0 to 16 years was classified into four age  
3  
4 groups: <1.5 years, 1.5 to 5.5 years, 5.5 to 10.5 years, and 10.5 to 16 years. This  
5  
6 age classification allowed the comparison of the actual Swiss practice in neuro-  
7  
8 paediatric CT to the earlier practice in Switzerland and in other countries.  
9

10  
11 For each child, we gathered the following data: 1. age; 2. date of the CT; 3.  
12  
13 indication for the CT; 4. exposure data, CTDI<sub>vol</sub>, and DLP, as well as approximated  
14  
15 scan length (SL) calculated by dividing the DLP by the CTDI<sub>vol</sub>; 5. number of scans (if  
16  
17 scans were repeated; e.g. because of lack of patient cooperation or excessive  
18  
19 motion). The values used for CTDI<sub>vol</sub> and the DLP were the displayed values.  
20  
21 Differences between the displayed and measured CTDI<sub>vol</sub> were in conformity with  
22  
23 Swiss legal requirements (limit of  $\pm 20\%$ ).  
24  
25  
26  
27

## 28 **2.2 CT indications**

29  
30 A consensus review between the study coordinator, the local physicists collecting the  
31  
32 data sets and the responsible person of the radiation protection authority of the  
33  
34 CTDI<sub>vol</sub> and DLP was undertaken for the following three anatomical regions: brain,  
35  
36 facial bone and petrous bone; each with and without contrast medium (CM)  
37  
38 application. All indications for cranial CT imaging were assigned to one of these  
39  
40 regions. The medical indications for these defined anatomical regions, each with and  
41  
42 without CM, are summarised in Table1.  
43  
44

45  
46 All paediatric neuro CTs analysed were indicated after explicit consultation with the  
47  
48 clinician and were of sufficient diagnostic image quality with regard to the clinical  
49  
50 question. None of the scans were acquired only for study purposes.  
51  
52  
53

## 54 **2.3 Patient data analysis**

55  
56  
57  
58  
59  
60

1  
2 The data acquired were analysed per centre, and stratified according to age group  
3  
4 and anatomical region; with and without CM. If more than one CT scan had to be  
5  
6 acquired for a patient, e.g. if the patient had moved or needed several follow-up CT  
7  
8 scans; each was evaluated separately.  
9

10  
11 For each age group, anatomic region and hospital, median values for  $CTDI_{vol}$   
12  
13 and DLP were calculated. Descriptive statistical analysis of the resulting distributions  
14  
15 of the median values yielded values for minimum, maximum, 25th percentile (1st  
16  
17 quartile), median (2nd quartile), and 75th percentile (3rd quartile). In accordance with  
18  
19 the recommendations of the ICRP [9], national DRLs were defined as the 75th  
20  
21 percentiles of the dose distributions.  
22  
23

24  
25 The results for brain CTs were compared with the currently valid DRLs in  
26  
27 Switzerland [20], from *L'Institut de Radioprotection et de Sûreté Nucléaire* (IRSN)  
28  
29 France 2009 [21], the American Association of Physicists in Medicine (AAPM) [22]  
30  
31 and the European Guidelines on DRLs for Paediatric Imaging [23]. For the  
32  
33 international comparison of the anatomic region of facial bone we used the available  
34  
35 valid DRLs from Switzerland [20] and the IRSN France [21] and, for petrous bone,  
36  
37 DRLs from the IRSN France [21], which were the only ones available. Our literature  
38  
39 search did not yield other comparable DRLs for the anatomic regions of facial bone  
40  
41 and petrous bone; in our experience the second and third most frequently CT-  
42  
43 examined anatomic regions in children. Note that the survey from *L'Institut de*  
44  
45 *Radioprotection et de Sûreté Nucléaire* (IRSN) France 2009 does not document  
46  
47 DRLs for children older than 10 years [21].  
48  
49  
50  
51

52  
53 Data were reviewed and processed by an experienced medical physicist, and  
54  
55 an independent quality assurance check of the processed data was performed. If  
56  
57 necessary, clarification from the project coordinator was requested. At the end of our  
58  
59  
60

1 study each of the participating centres received a copy of their recorded data to verify  
2 whether the data were correct and if any comments needed to be added.  
3  
4

### 5 **Statistical analysis**

6  
7  
8 The statistical analysis was performed using R software version 3.3.3 (R: A language  
9 and environment for statistical computing. R Foundation for Statistical Computing,  
10 Vienna, Austria). The statistical significance of differences between the different age  
11 groups for each anatomical localisation was tested with Kruskal-Wallis (significance  
12 level  $p = 0.05$ ).  
13  
14  
15  
16  
17  
18  
19  
20  
21

## 22 **3. Results**

23  
24 In total, 1645 (100%) paediatric neuro CTs were recorded and retrospectively  
25 analysed: 1172 (71.2%) brain CTs without CM application; 127 (7.7%) brain CTs with  
26 CM application; 206 (12.5%) facial bone CTs without CM application; 14 (0.9%) facial  
27 bone CTs with CM application, 125 (7.6%) petrous bone CTs without CM application  
28 and 1 (0.1%) petrous bone CT with CM application. The total frequencies of all types  
29 of examination are given in Table 2.  
30  
31  
32  
33  
34  
35  
36  
37

38 The number of CTs with CM application was very low; dose data for CTs with  
39 and without CM application for the three anatomic regions (results in the appendix)  
40 were pooled for further analysis. For most of the studies with CM application the  
41 same CT protocol with the same scanning parameters were used as for native CT  
42 studies. In Table 3, the 75th percentiles of the distribution of the median values of all  
43 eight centres for  $CTDI_{vol}$  and DLP are presented for the three anatomic regions. The  
44 values for  $CTDI_{vol}$  and DLP recorded for each centre separately are documented in  
45 the appendix.  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55

56 The comparison of the 75th percentiles of the distribution of the median values  
57 of all eight centres for  $CTDI_{vol}$  and DLP for brain CTs to the currently valid DRLs in  
58  
59  
60

1  
2 Switzerland [20], from IRSN France [21], the AAPM [22] and the European  
3  
4 Guidelines on DRLs for Paediatric Imaging [23] revealed from 10% up to 40% lower  
5  
6 values; compare Fig. 1a and 1b. The international comparison of the anatomic  
7  
8 regions, facial bone and petrous bone, with the available valid DRLs for facial bone  
9  
10 from Switzerland [20] and the IRSN France [21] and with the available DRLs from the  
11  
12 IRSN France [21] for petrous bone, also revealed decreases in the 75th percentiles  
13  
14 from 5% to 70% in comparison to the currently valid values as shown in Figs 2a and  
15  
16 2b and Figs 3a and 3b.  
17  
18  
19

20 For  $CTDI_{vol}$ , there was a significant difference between the age classes for the  
21  
22 brain ( $p < 0.001$ ) and the facial bone ( $p < 0.05$ ), but not for the petrous bone ( $p =$   
23  
24  $0.24$ ). Concerning the DLP value, significant differences between age classes were  
25  
26 found for the brain ( $p < 0.001$ ), the facial bone ( $p = 0.01$ ) and the petrous bone ( $p =$   
27  
28  $0.02$ ).  
29  
30  
31

32 In contrast, the SL for the three anatomical regions was higher than the  
33  
34 currently valid values in Switzerland [20], as well as those from IRSN France [21], the  
35  
36 AAPM [22], and the European Guidelines on DRLs for Paediatric Imaging [23] (see  
37  
38 appendix).  
39  
40

41 In our large cohort of CTs, no wide variations in dose were found between the  
42  
43 participating hospitals (compare appendix).  
44  
45

46 New DRLs for neuro-paediatric CT examinations in Switzerland were based  
47  
48 on the 75th percentiles of the distributions of the median values of all eight centres.  
49  
50 Where appropriate, values were rounded such that the DRLs increase, or at least  
51  
52 remain constant, as the age of the patient increases. From our point of view such  
53  
54 rounding of the values is practical for hospitals acquiring paediatric CTs. Table 4  
55  
56 shows the rounded values that were obtained taking the standard deviations into  
57  
58  
59  
60

1  
2 consideration. The new proposed DRLs for the three anatomic regions – brain, facial  
3  
4 bone and petrous bone – are presented in Table 4 and Figs 4a and 4b.  
5  
6  
7  
8  
9

#### 10 11 **4. Discussion**

12  
13 Following our study, we established new age-related DRLs for  $CTDI_{vol}$  and DLP for  
14  
15 the most frequently performed neuro-paediatric CT examinations in Switzerland. Our  
16  
17 results with new DRLs for  $CTDI_{vol}$  and DLP up to 20% lower than the DRLs so far  
18  
19 used in Switzerland, as well as in other European countries (Figs 1 to 3), confirm the  
20  
21 importance of regular re-assessment of the radiological practice; at least every 3 to  
22  
23 (maximum) 5 years. As a consequence of our study, new national DRLs were  
24  
25 established in Switzerland for  $CTDI_{vol}$  and DLP for paediatric patients in four defined  
26  
27 age groups (<1.5 years, 1.5 to 5.5 years, 5.5 to 10.5 years and 10.5 to 16 years) for  
28  
29 the three main anatomic regions – brain, facial bone and petrous bone.  
30  
31  
32  
33

34 DRLs are considered to be dynamic values that are reviewed periodically [24].  
35  
36 DRLs for indication-based CTs in Switzerland were established for adults in 2010  
37  
38 [25]. Results showed large variations in doses between different radiology  
39  
40 departments in Switzerland, especially for examinations of the petrous bone, pelvis,  
41  
42 lower limbs and heart, indicating that the concept of DRLs was not being correctly  
43  
44 applied for CTs in clinical routine in Switzerland.  
45  
46  
47

48 A dose optimisation process should be triggered resulting in a lower radiation  
49  
50 dose, especially in children. By repeatedly implementing such reviews, the global  
51  
52 radiation dose is expected to decrease over a (short) period of time [15,25–29].  
53  
54

55 As our study demonstrated, a multidisciplinary collaboration between different  
56  
57 centres is essential when developing and implementing dose-optimised CT protocols  
58  
59  
60

1  
2 beyond institutional single-centre boundaries. As shown, each participating centre  
3  
4 provided a different amount of CT data depending on the hospital's size.  
5

6 Since there was no statistically significant difference between dose data with  
7  
8 and without CM application for the three defined anatomic regions and the number of  
9  
10 CTs with CM was very low, the dose data were pooled for analysis. This decision  
11  
12 was supported by the data evaluation, which revealed that for most of the studies  
13  
14 with CM the same CT protocol was used with the same scanning parameters as for  
15  
16 native CT studies. The pooling increased the statistical power and led to more  
17  
18 reliable results.  
19  
20  
21

22 The routine use of dose management software during CT scanning might also  
23  
24 have an influence on the results. Centres using commercial or in-house developed  
25  
26 dose management software provided more data than centres collecting dose data  
27  
28 manually. The new Swiss DRLs for  $CTDI_{vol}$  and DLP are much lower than the current  
29  
30 Swiss DRLs and the DRLs of other European countries, indicating the use of dose-  
31  
32 optimised CT protocols. Nevertheless, SLs were slightly higher than current values  
33  
34 and the DRLs of other European countries suggesting a non-optimised radiological  
35  
36 practice. The scan range chosen was too conservative and emphasises the need for  
37  
38 continuation of efforts towards the optimisation of CT protocols.  
39  
40  
41  
42

43 Radiation dose must not be the only criterion considered when choosing the  
44  
45 appropriate imaging modality for children. Some of the indications listed in Table 1  
46  
47 could be examined adequately with MRI. But MRI is not always practical or  
48  
49 preferable: particularly in acute trauma patients needing rapid treatment, CT is the  
50  
51 preferred modality. Therefore, it is important to have CT protocols in place that  
52  
53 minimise radiation dose without sacrificing diagnostic accuracy. Unfortunately, in  
54  
55 practice, DRLs have not changed significantly over time [24]. Even though DRLs are  
56  
57  
58  
59  
60



1  
2 currently the best tools for dose optimisation, the concept of DRLs only seems to  
3  
4 work slowly. The DRL values set by different countries for brain CT examinations in  
5  
6 children have changed little in recent years; several countries published current  
7  
8 DRLs (2010–2014) that are equal to or even higher than the initial paediatric DRLs  
9  
10 [24]. Although the ALARA principle is now more than 35 years old [30], and was  
11  
12 introduced in paediatric imaging more than 10 years ago [8], it seems that there is  
13  
14 still work to be done on dose optimisation in paediatric brain CT scans. This is  
15  
16 highlighted by our current results with DRLs for  $CTDI_{vol}$  and DLP up to 20% lower  
17  
18 than the DRLs so far used in Switzerland as in other European countries.  
19  
20  
21

22  
23 There is no doubt that such regular data collection and re-evaluation is time  
24  
25 and resource consuming, but since the Swiss legislation demands the  
26  
27 implementation of DRLs and since dose management systems are increasingly  
28  
29 installed in radiology departments allowing automatic data collection, this will  
30  
31 facilitate such an endeavour.  
32  
33

34  
35 A major element of that process of optimisation is a national and international  
36  
37 consensus on the DRLs to avoid wide variations and minimise radiation risk and  
38  
39 long-term complications in children. We recommend a timeframe of 3 to a maximum  
40  
41 of 5 years. In future, it would be worthwhile to suggest DRLs for sub-specific cranial  
42  
43 CT indications that might have different image quality requirements.  
44  
45  
46  
47

## 48 **5. Limitations**

49  
50 The number of paediatric cranial CTs performed in Switzerland is limited. There are  
51  
52 relatively few paediatric patients owing the small population and low number of  
53  
54 university, cantonal and regional hospitals compared to other European countries.  
55  
56  
57  
58  
59  
60

1  
2 The small amount of dose data inevitably results in decreased statistical accuracy.

3  
4 However, since one of the aims of this study was to harmonise the CT practice  
5  
6 across Switzerland, all available data was included for analysis.  
7  
8  
9

10  
11 We are also aware that the different methods of data collection in the eight hospitals  
12  
13 – using commercial dose management software; in-house developed data collection  
14  
15 or manual data registration in specific spreadsheets – might have an influence on the  
16  
17 amount and correctness of collected data. Commercial dose management software  
18  
19 accesses all dose data from the DICOM header whereas manual data collection  
20  
21 might be biased in terms of number and accuracy.  
22  
23  
24

25 To improve statistical accuracy, the calculation of the 75th percentile of a dose  
26  
27 distribution should be based on at least 20 data sets, as recommended by the ICRP  
28  
29 in publication 135 on DRLs in medical imaging [9]. However, since the number of  
30  
31 neuro-paediatric CT scans in Switzerland is limited, several hospitals provided many  
32  
33 fewer than 20 data sets for specific examinations (see Table 2). If these data were to  
34  
35 be omitted from the analysis, DRLs would be based on data from only a few hospitals  
36  
37 and would not reflect the overall CT practice across Switzerland. Therefore, in order  
38  
39 to harmonise the CT practice across Switzerland, we decided to include all data in  
40  
41 our analysis, being fully aware that the statistical accuracy was decreased.  
42  
43  
44

45 Image quality of the CT scans was assessed in a qualitative manner by the clinicians  
46  
47 depending on the clinical indication. Image quality was considered to be sufficient if it  
48  
49 allowed an accurate diagnosis. No quantitative image quality assessment (e.g. by  
50  
51 calculating the signal-to-noise ratio or using model observers) was performed, since  
52  
53 this would have gone beyond the scope of this study.  
54  
55  
56  
57  
58  
59  
60

## 6. Conclusion

This article reports results from a national dose survey of neuro-paediatric CT examinations (1645 data sets were analysed) in eight participating university and cantonal hospitals in Switzerland. Results with DRLs for  $CTDI_{vol}$  and DLP up to 20% lower than the DRLs so far used in Switzerland and other European countries, indicate that regular national and international updates of DRLs are essential. With respect to the rapidly evolving technology allowing a lower exposure to radiation while maintaining a high image quality sufficient for a correct diagnosis, periodic updates of regional and international DRLs at least every 3 to a maximum of 5 years are indispensable to establish optimum conditions for paediatric brain CTs.

## Acknowledgements

We would like to thank the eight participating hospitals; the university hospitals of Geneva, Lausanne, Bern, Basel and Zurich and the cantonal hospitals of Chur, Aarau and Lucerne for providing the neuro-paediatric CT data sets.

## References

1. Larson DB, Johnson LW, Schnell BM, et al. Rising use of CT in child visits to the emergency department in the United States, 1995-2008. *Radiology*. 2011;259:793–801.
2. Fearon JA, Singh DJ, Beals SP, et al. The diagnosis and treatment of single-sutural synostoses: are computed tomographic scans necessary? *Plast Reconstr Surg*. 2007;120:1327–31.
3. Jaffurs D, Denny A. Diagnostic pediatric computed tomographic scans of the head: actual dosage versus estimated risk. *Plast Reconstr Surg*. 2009;124:1254–60.
4. Morton RP, Reynolds RM, Ramakrishna R, et al. Low-dose head computed tomography in children: a single institutional experience in pediatric radiation risk reduction: clinical article. *J Neurosurg Pediatr*. 2013;12:406–10.
5. Pearce MS, Salotti JA, Little MP et al Radiation exposure from CT scans in childhood and subsequent risk of leukaemia and brain tumours: a retrospective cohort study. *Lancet*. 2012;380:499–505.
6. Mathews JD, Forsythe AV, Brady Z et al Cancer risk in 680, 000 people exposed to computed tomography scans in childhood or adolescence: data linkage study of 11 million Australians. *BMJ*. 2013;346:f2360.
7. United Nations Scientific Committee on the Effects of Atomic Radiation; UNSCEAR. Sources, effects and risk of ionizing radiation. Report to the General Assembly with Scientific Annexes. Vol. I. 2013. [http://www.unscear.org/unscear/en/publications/2013\\_1.html](http://www.unscear.org/unscear/en/publications/2013_1.html). Accessed 14 Nov 2017.
8. Slovis TL The ALARA concept in pediatric CT: myth or reality? *Radiology*. 2002; 223:5–6.
9. International Commission on Radiological Protection. Diagnostic reference levels in medical imaging. ICRP Publication 135. *Ann. ICRP* 2017; 46(1).
10. Directorate-General, Environment, Nuclear Safety and Civil Protection, European Commission. Radiation protection 109: guidance on diagnostic reference levels (DRLs) for medical exposures (radiation protection). 1999. [http://ec.europa.eu/energy/nuclear/radiation\\_protection/doc/publication/109\\_en.pdf](http://ec.europa.eu/energy/nuclear/radiation_protection/doc/publication/109_en.pdf).
11. Verdun FR, Gutierrez D, Vader JP et al CT radiation dose in children: a survey to establish age-based diagnostic reference levels in Switzerland. *Eur Radiol*. 2008;18:1980–86.

12. Galanski M, Nagel HD, Stamm G Results of a federation inquiry 2005/2006: pediatric CT X-ray practice in Germany. *Röfo*. 2007;179:1110–11.
13. Brisse HJ, Aubert B CT exposure from pediatric MDCT: results from the 2007-2008 SFIPP/ISRN survey. *J Radiol*. 2009;90:207–15.
14. Buls N, Bosmans H, Mommaert C et al. Current status on pediatric CT doses: a multicentre study (Belgium). RSNA meeting, Chicago. 2009.  
[www.fanc.fgov.be/GED/00000000/2400/2449.pdf](http://www.fanc.fgov.be/GED/00000000/2400/2449.pdf). Accessed 14 Nov 2017.
15. Federal Office for Radiation Protection. Notice of diagnostic reference levels for radiology and nuclear medicine examinations. [In German.] Salzgitter, Germany: Federal Office for Radiation Protection; 2010.
16. Larson DB, Johnson LW, Schnell BM, Goske MJ, Salisbury SR, Forman HP Rising use of CT in child visits to the emergency department in the United States, 1995-2008. *Radiology*. 2011;259:793–801.
17. Larson DB, Molvin LZ, Wang J, Chan FP, Newman B, Fleischmann D Pediatric CT quality management and improvement program. *Pediatr Radiol*. 2014;44(Suppl 3):519–24.
18. Watson DJ, Coakley KS Paediatric CT reference doses based on weight and CT dosimetry phantom size: local experience using a 64-slice CT scanner. *Pediatr Radiol*. 2010;40:693–703.
19. Pages J, Buls N, Osteaux MCT doses in children: a multicentre study. *Br J Radiol* . 2003;76:803–11.
20. Verdun FR, Gutierrez D, Vader JP et al CT radiation dose in children: a survey to establish age-based diagnostic reference levels in Switzerland. *Eur Radiol*. 2008;18:1980–86.
21. Société Française de Radiologie. Guide pratique à l'usage des médecins radiologues pour l'évaluation de leurs pratiques professionnelles. Paris: Société Française de Radiologie; 2009.
22. AAPM. American Association of Physicists in Medicine. Use of water equivalent diameter for calculating patient size and size-specific dose estimates (SSDE) in CT, AAPM Report No. 220. College Park, MD: American Association of Physicists in Medicine; 2014.
23. European Commission (EC). European Guidelines on DRLs for paediatric imaging. 2015. (draft) <http://www.eurosafeimaging.org/wp/wp-content/uploads/2015/09/European->

1  
2 Guidelines-on-DRLs-for-Paediatric-Imaging\_FINAL-for-workshop\_30-Sept-2015.pdf.

3  
4 Accessed 14 Nov 2017.

5  
6 24. De Bondt T, Mulkens T, Zanca F, Pyfferoen L, Casselman JW, Parizel PM.  
7 Benchmarking pediatric cranial CT protocols using a dose tracking software system: a  
8 multicenter study. *Eur Radiol.* 2017;27:841–50.

9  
10  
11 25. Treier R, Aroua A, Verdun FR, Samara E, Stuessi A, Trueb PR Patient doses in CT  
12 examinations in Switzerland: implementation of national diagnostic reference levels. *Radiat*  
13 *Prot Dosim.* 2010;142:244–54.

14  
15  
16  
17 26. Shrimpton PC, Hillier MC, Meeson S and Golding SJ. Doses from computed tomography  
18 (CT) examinations in the UK – 2011 review.  
19 [https://www.gov.uk/government/uploads/system/uploads/attachment\\_data/file/349188/PHE\\_](https://www.gov.uk/government/uploads/system/uploads/attachment_data/file/349188/PHE_CRCE_013.pdf)  
20 [CRCE\\_013.pdf](https://www.gov.uk/government/uploads/system/uploads/attachment_data/file/349188/PHE_CRCE_013.pdf). Accessed 14 Nov 2017.

21  
22  
23  
24 27. Roch P, Aubert B French diagnostic reference levels in diagnostic radiology, computed  
25 tomography and nuclear medicine: 2004-2008 review. *Radiat Prot Dosim.* 2013;154:52–75.

26  
27  
28 28. Australian Radiation Protection and Nuclear Safety Agency national diagnostic reference  
29 level fact sheet. 2013. <http://www.arpansa.gov.au/services/ndrl/adult.cfm>. Accessed 14 Nov  
30 2017.

31  
32  
33 29. Dosimétrie de patients en radiologie, Belgium 2014 (French).  
34 [http://www.fanc.fgov.be/fr/page/dosimetrie-despatients-en-radiologie/1196.aspx#P\\_8196](http://www.fanc.fgov.be/fr/page/dosimetrie-despatients-en-radiologie/1196.aspx#P_8196).

35  
36  
37 30. Winkler NT ALARA concept—now a requirement. *Radiol Technol.* 1980;51:525.

38  
39  
40 31. World Medical Association Declaration of Helsinki. Ethical principles for medical research  
41 involving human subjects. <http://jama.jamanetwork.com/article.aspx?articleid=1760318>,  
42 Accessed 12 Aug 2015.  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15

## TABLES

16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26

### Table 1

Indications for cranial computed tomography (CT) imaging in paediatrics assigned to the three anatomic subgroups: brain, facial bone and petrous bone, with and without contrast medium (CM).

27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

Anatomical Region	Medical Indication
Brain without CM application	<ul style="list-style-type: none"> <li>• brain trauma</li> <li>• child abuse</li> <li>• evaluation of ventricular width (e.g. in patients with suspected shunt dysfunction)</li> <li>• localisation of brain pressure probes</li> <li>• preoperative determination of extent of craniosynostosis</li> <li>• dysmorphia of the skull</li> <li>• detection and evaluation of calcifications (e.g. in syndromes such as Sturge-Weber)</li> </ul>
Brain with CM application	<ul style="list-style-type: none"> <li>• in complicated mastoiditis to rule out intracranial complications like sinus vein thrombosis, intracranial abscess, or Bezold's abscess</li> <li>• central and anterior skull-base tumours (e.g. fibrous dysplasia, ossifying fibroma, ecchordis physalliphora)</li> <li>• for staging of systemic diseases like Langerhans histiocytosis or mastocytosis with multifocal brain manifestations</li> </ul>
Facial bone without CM application	<ul style="list-style-type: none"> <li>• midface trauma (fracture evaluation) including the paranasal sinus, nose and orbit</li> <li>• choanal atresia and stenosis of piriform aperture</li> <li>• polyposis nasi, Morbus Widal and evaluation of uncomplicated sinusitis</li> <li>• dentogenic pathologies (e.g. periradicular cysts)</li> <li>• for foreign body localisation after midface trauma or in case of ingestion</li> <li>• juvenile temporomandibular arthropathy</li> </ul>
Facial bone with CM application	<ul style="list-style-type: none"> <li>• complicated sinusitis</li> <li>• acute and chronic osteomyelitis of midface and anterior skull, as well as recurrent infections (e.g. recurrent multifocal osteomyelitis in children)</li> <li>• osteonecrosis (e.g. radiogenic induced)</li> <li>• suspected nasal, paranasal or orbital tumours</li> <li>• tumour-like lesions and temporomandibular joint tumours (e.g. chondromatosis)</li> </ul>
Petrous bone without CM application	<ul style="list-style-type: none"> <li>• congenital anomalies of the temporal bone, middle ear cavity, and inner ear</li> <li>• for postoperative cochlear implant location, or localisation of hearing aids</li> </ul>
Petrous bone with CM application	<ul style="list-style-type: none"> <li>• in complicated mastoiditis to rule out periauricular complications like Bezold's abscess</li> <li>• posterior skull-base tumours (e.g. fibrous dysplasia, ossifying fibroma)</li> </ul>

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

	<ul style="list-style-type: none"><li>• staging of systemic diseases like Langerhans histiocytosis or mastocytosis with focal posterior skull-base manifestation</li><li>• acute or chronic osteomyelitis, as well as recurrent infections of posterior skull-base</li></ul>
--	--



**Table 2**

Total frequencies of all types of examinations at all eight participating centres.

<b>Centres</b>	<b>Brain without CM</b>	<b>Brain with CM</b>	<b>Facial Bone without CM</b>	<b>Facial Bone with CM</b>	<b>Petrous Bone without CM</b>	<b>Petrous Bone with CM</b>	<b>Total number of CT's</b>	<b>Total % of CT's</b>
<b>A</b>	149	16	34	4	23	1	<b>227</b>	<b>14</b>
<b>B</b>	130	31	18	2	17	0	<b>198</b>	<b>12</b>
<b>C</b>	17	0	5	1	3	0	<b>26</b>	<b>2</b>
<b>D</b>	38	0	4	1	9	0	<b>52</b>	<b>3</b>
<b>E</b>	28	11	2	1	9	0	<b>51</b>	<b>3</b>
<b>F</b>	39	10	29	3	21	0	<b>102</b>	<b>6</b>
<b>H</b>	309	25	47	0	0	0	<b>381</b>	<b>23</b>
<b>I</b>	462	34	67	3	43	0	<b>609</b>	<b>37</b>
<b>Total number of CT's</b>	1172	127	206	14	125	1	<b>1645</b>	-
<b>Total % of CT's</b>	71.2%	7.7%	12.5%	0.9%	7.6%	0.1%	-	<b>100</b>

**Table 3**

The new proposed rounded DRLs (75th percentiles) and the target values (median values) for CTDI<sub>vol</sub> and DLP for neuro-paediatric CT examinations, age-related and separated according to the three anatomic regions: brain, facial bone and petrous bone. For CTDI<sub>vol</sub> compare Fig. 4a and for DLP compare Fig. 4b.

Anatomical region	Patient's age [years]	DRLs (75th percentile)		Target value (median)	
		CTDI <sub>vol</sub> [mGy]	DLP [mGy.cm]	CTDI <sub>vol</sub> [mGy]	DLP [mGy.cm]
<b>Brain</b> without and with CM	< 1.5	25	350	20	300
	1.5–5.5	30	420	24	390
	5.5–10.5	35	540	30	490
	> 10.5	40	670	36	610
<b>Facial Bone</b> without and with CM	< 1.5	10	120	7	90
	1.5–5.5	10	120	7	90
	5.5–10.5	15	170	7	110
	> 10.5	15	200	10	140
<b>Petrous Bone</b> without and with CM	< 1.5	20	110	17	95
	1.5–5.5	30	200	20	110
	5.5–10.5	30	200	20	150
	> 10.5	30	200	20	150

**FIGURES**

**Fig. 1** Comparison of the 75th percentiles for CTDI<sub>vol</sub> (Fig. 1a) and DLP (Fig. 1b) for brain CT scans (black bars) compared to the currently valid DRLs in Switzerland from 2010 and in France from 2009 as well as to the DRLs published by the AAPM in 2014 and by the European Commission in 2015.

Fig. 1a


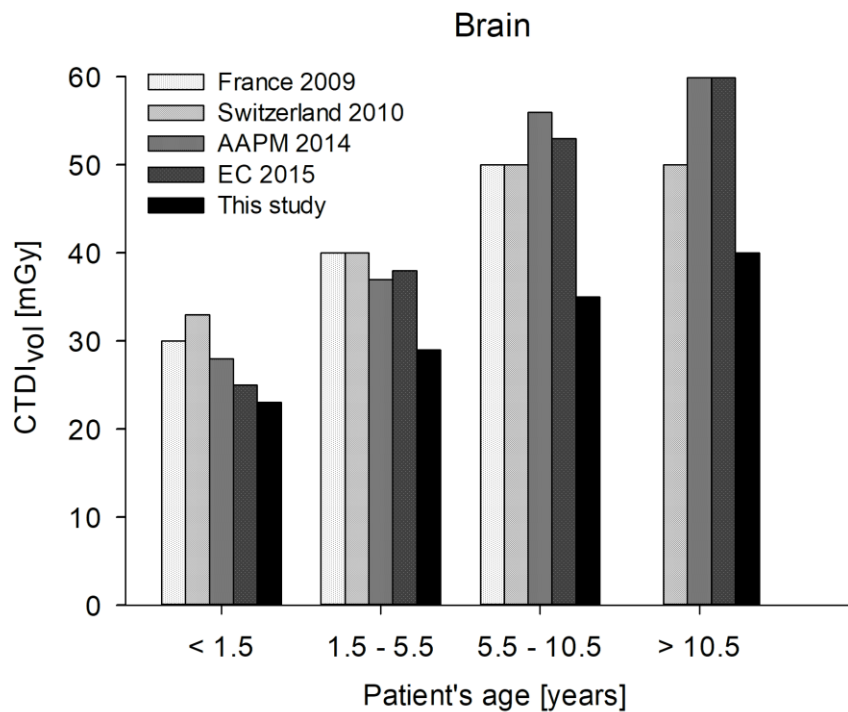


Fig. 1b

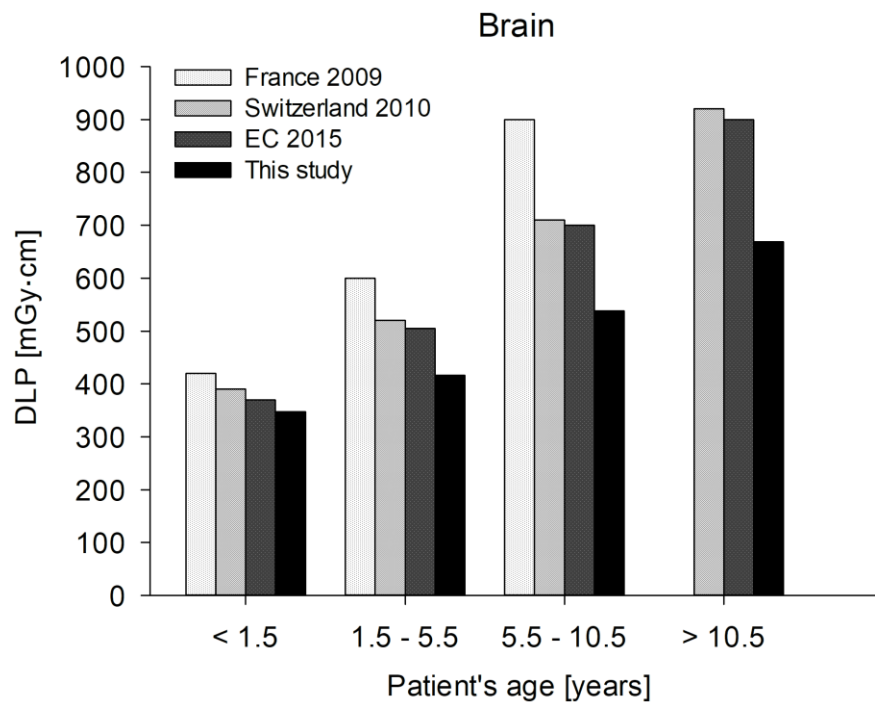

1  
2 **Fig. 2** Comparison of the 75th percentiles for  $CTDI_{vol}$  (Fig. 2a) and DLP (Fig. 2b) for  
3  
4 facial bone CT scans (black bars) compared to the currently valid DRLs in  
5  
6 Switzerland from 2010 and in France from 2009.  
7  
8  
9

10  
11 Fig. 2a  
12  
13  
14  
15  
16  
17


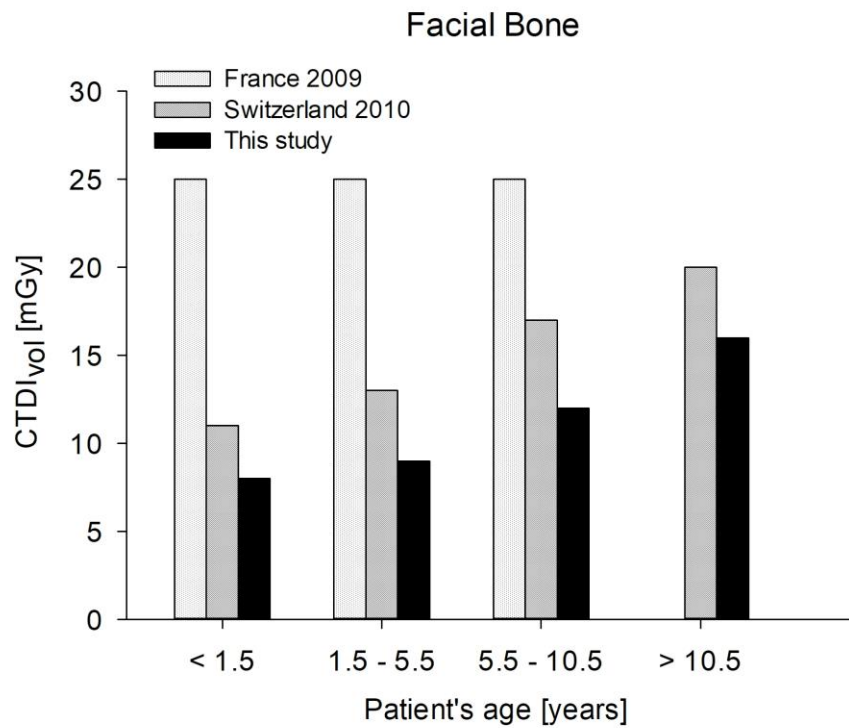


Fig. 2b

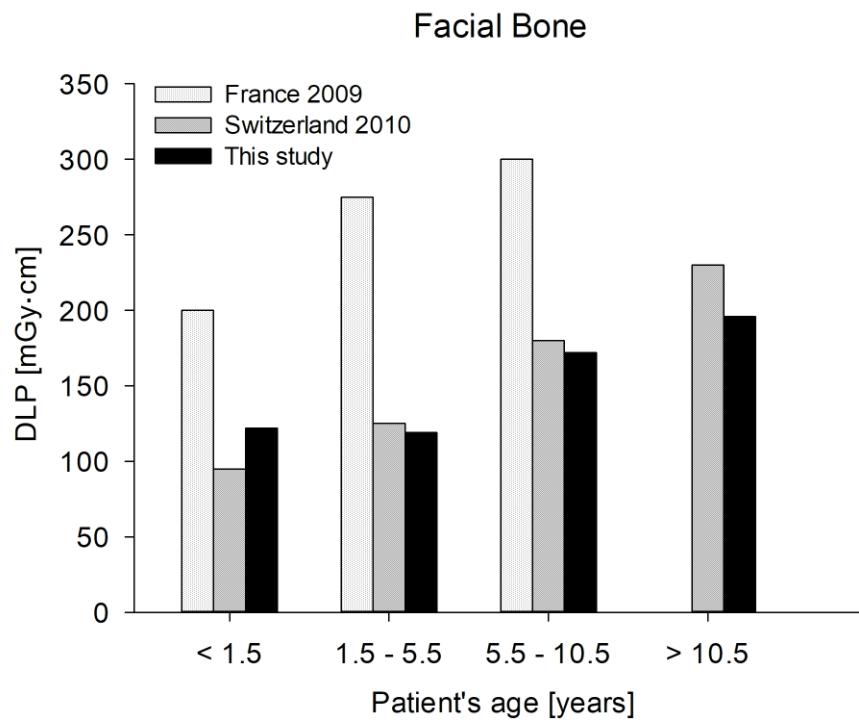

1  
2 **Fig. 3** Comparison of the 75th percentiles for  $CTDI_{vol}$  (Fig. 3a) and DLP (Fig. 3b) for  
3  
4 petrous bone CT scans (black bars) compared to the currently valid DRLs in France  
5  
6 from 2009.  
7  
8  
9

10  
11 Fig. 3a  
12  
13  
14  
15  
16  
17  
18

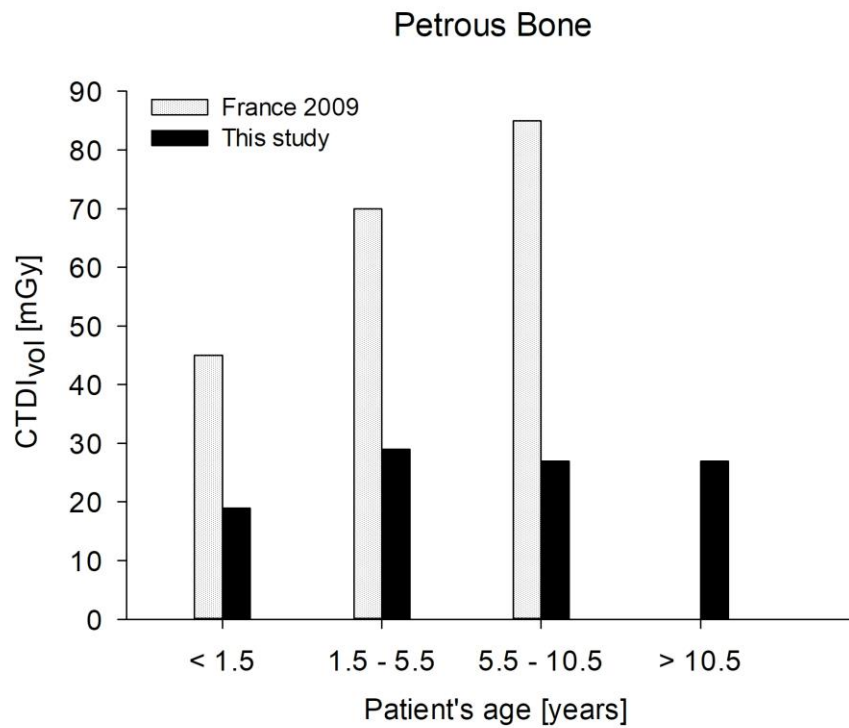
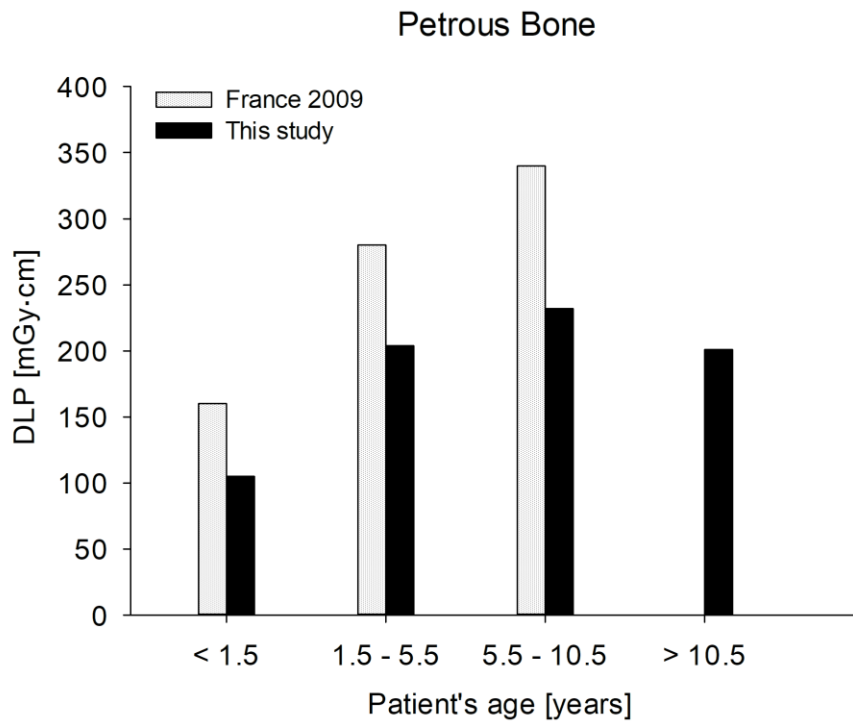


Fig. 3b





**Fig. 4** The proposed new rounded DRLs (grey bars) based on the 75th percentiles (in brackets) for  $CTDI_{vol}$  (Fig. 4a) and DLP (Fig. 4b) for neuro-paediatric CT examinations; age-related and separated according to the three anatomic regions: brain, facial bone and petrous bone.

Fig. 4a


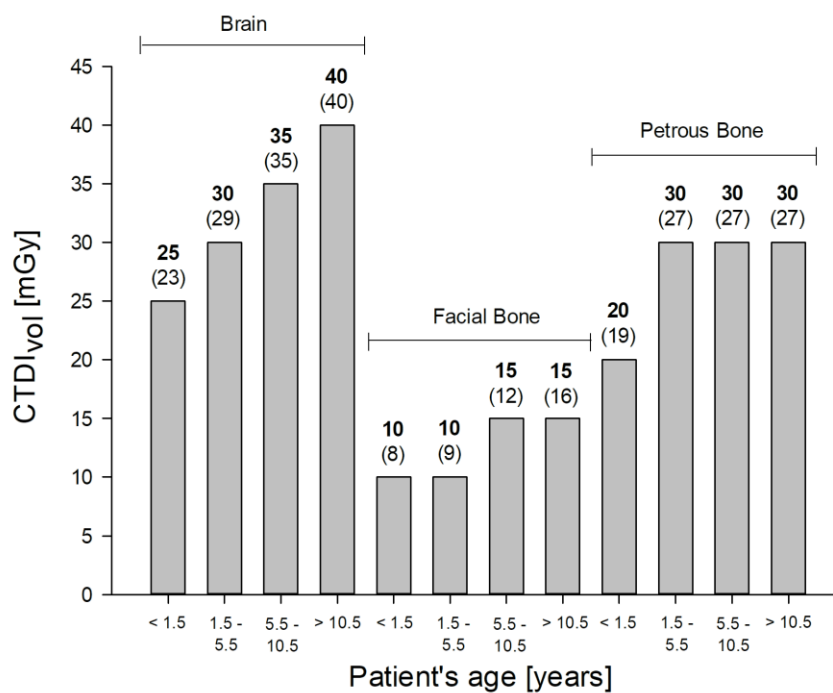


Fig. 4b

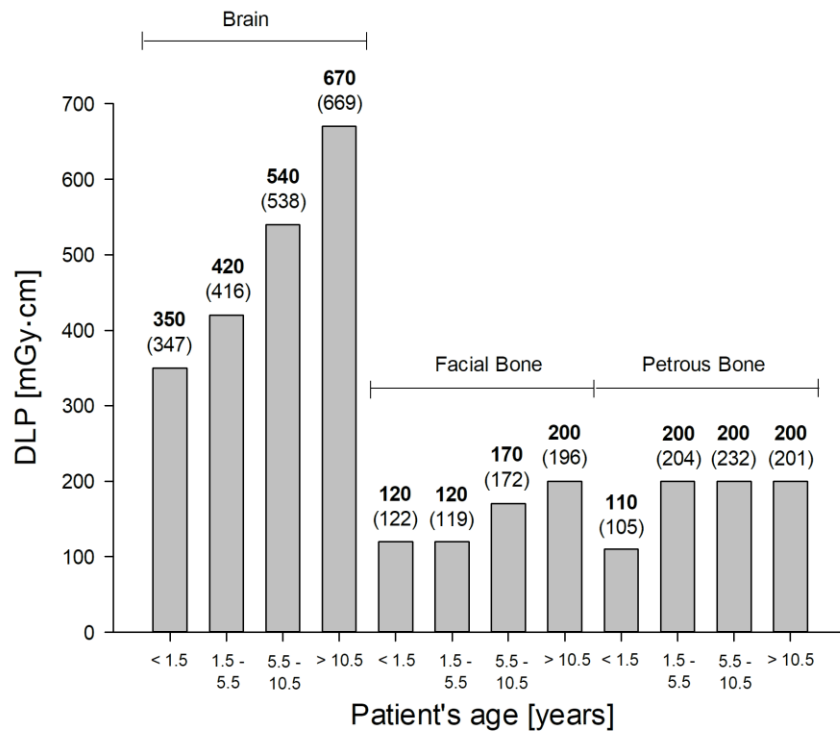

## APPENDIX

**A: Median values for CTDI<sub>vol</sub>, DLP and scan length from all eight centres for CT of the brain with and without primary CM application separated by age group.**

Table A.1 Paediatric Patients aged &lt;1.5 years, brain CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	17	6	13	17	5	6	12	1	1	
	25 <sup>th</sup> percentile	18	16	13	20	10	8	14	1	13	
	<b>Median</b>	30	23	13	20	13	20	16	16	16	<b>21</b>
	75 <sup>th</sup> percentile	31	26	13	22	13	24	19	16	19	
	Max	32	30	13	26	21	26	27	29	32	
DLP [mGy.cm]	Min	241	18	207	255	108	66	31	25	18	
	25 <sup>th</sup> percentile	292	202	209	307	151	134	205	30	163	
	<b>Median</b>	474	314	211	321	186	299	245	182	229	<b>316</b>
	75 <sup>th</sup> percentile	530	361	212	339	201	365	273	231	290	
	Max	723	416	214	395	417	483	390	628	723	
Scan length [cm]	Median	16	14	16	15	16	15	15	14	15	<b>16</b>
number of exams		26	38	2	10	5	11	64	107	263	

Table A.2 Paediatric patients aged &lt;1.5 years, brain CT with CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	32	22	n	n	n	22	14	16	12	
	25 <sup>th</sup> percentile	32	25	n	n	n	22	14	16	16	
	<b>Median</b>	32	26	n	n	n	22	14	16	20	<b>26</b>
	75 <sup>th</sup> percentile	32	26	n	n	n	22	14	16	26	
	Max	32	27	n	n	n	22	14	16	32	
DLP [mGy.cm]	Min	321	120	n	n	n	347	181	136	22	
	25 <sup>th</sup> percentile	366	630	n	n	n	347	190	189	197	
	<b>Median</b>	410	679	n	n	n	347	199	197	236	<b>410</b>
	75 <sup>th</sup> percentile	455	816	n	n	n	347	208	221	320	
	Max	500	943	n	n	n	347	217	251	500	
Scan length [cm]	Median	13	13	n	n	n	16	14	12	13	<b>14</b>
number of exams		2	8	0	0	0	1	2	7	20	

Table A.3 Paediatric patients aged 1.5 to 5.5 years, brain CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	18	12	16	15	6	24	16	1	1	
	25 <sup>th</sup> percentile	31	28	16	20	11	25	19	19	19	
	<b>Median</b>	32	30	16	22	17	26	25	19	19	<b>27</b>
	75 <sup>th</sup> percentile	32	30	21	24	17	27	35	19	30	
	Max	32	44	26	27	17	30	39	40	44	
DLP [mGy.cm]	Min	189	22	276	246	77	391	159	13	13	
	25 <sup>th</sup> percentile	530	390	276	339	188	396	301	252	271	
	<b>Median</b>	577	416	276	366	300	401	435	271	312	<b>420</b>
	75 <sup>th</sup> percentile	630	472	360	426	307	436	515	290	472	
	Max	803	870	443	521	314	528	932	577	932	
Scan length [cm]	Median	18	14	18	18	18	16	16	14	15	<b>18</b>
number of exams		31	44	3	19	3	4	69	118	291	

Table A.4 Paediatric patients aged 1.5 to 5.5 years, brain CT with CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	31	16	n	n	5	25	19	14	5	
	25 <sup>th</sup> percentile	31	29	n	n	11	26	19	18	19	
	<b>Median</b>	31	30	n	n	17	26	19	19	27	<b>29</b>
	75 <sup>th</sup> percentile	32	32	n	n	18	26	31	19	31	
	Max	32	43	n	n	18	31	36	19	43	
DLP [mGy.cm]	Min	499	43	n	n	89	331	263	252	43	
	25 <sup>th</sup> percentile	551	345	n	n	210	401	277	266	293	
	<b>Median</b>	596	416	n	n	331	409	313	271	405	<b>414</b>
	75 <sup>th</sup> percentile	666	454	n	n	356	410	480	298	454	
	Max	791	529	n	n	381	446	556	382	791	
Scan length [cm]	Median	19	14	n	n	20	16	15	14	16	<b>18</b>
number of exams		4	8	0	0	3	5	6	4	30	

Table A.5 Paediatric patients aged 5.5 to 10.5 years, brain CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	29	28	4	16	6	11	4	1	1	
	25 <sup>th</sup> percentile	31	30	11	21	14	26	28	33	28	
	<b>Median</b>	32	31	18	21	17	28	36	35	32	<b>33</b>
	75 <sup>th</sup> percentile	32	35	20	23	18	31	46	36	36	
	Max	32	39	30	28	21	33	50	41	50	
DLP [mGy.cm]	Min	381	390	51	297	54	254	36	16	16	
	25 <sup>th</sup> percentile	522	416	186	349	193	429	468	473	452	
	<b>Median</b>	594	500	285	365	262	462	550	510	511	<b>520</b>
	75 <sup>th</sup> percentile	683	543	329	392	309	553	719	547	583	
	Max	923	621	533	504	385	614	983	838	983	
Scan length [cm]	Median	19	15	16	17	16	17	16	15	16	<b>17</b>
number of exams		32	12	5	7	4	17	73	114	264	

Table A.6 Paediatric patients aged 5.5 to 10.5 years, brain CT with CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	30	29	n	n	19	27	28	19	15	
	25 <sup>th</sup> percentile	31	29	n	n	20	28	28	35	28	
	<b>Median</b>	32	29	n	n	22	29	36	36	32	<b>35</b>
	75 <sup>th</sup> percentile	32	29	n	n	27	29	48	36	36	
	Max	32	29	n	n	37	30	48	40	48	
DLP [mGy.cm]	Min	261	472	n	n	326	460	418	271	216	
	25 <sup>th</sup> percentile	503	472	n	n	378	468	482	510	473	
	<b>Median</b>	560	472	n	n	431	476	515	546	511	<b>538</b>
	75 <sup>th</sup> percentile	721	472	n	n	538	484	707	583	613	
	Max	778	472	n	n	755	491	815	659	815	
Scan length [cm]	Median	18	16	n	n	19	17	15	15	16	<b>18</b>
number of exams		8	1	0	0	4	2	7	17	39	

Table A.7 Paediatric patients aged 10.5 to 16 years, brain CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	29	23	26	19	4	23	23	1	1	
	25 <sup>th</sup> percentile	31	39	26	22	8	30	36	39	31	
	<b>Median</b>	32	45	39	24	17	32	46	40	40	<b>41</b>
	75 <sup>th</sup> percentile	32	45	39	26	20	34	50	40	41	
	Max	46	53	40	29	27	41	174	41	174	
DLP [mGy.cm]	Min	357	451	416	363	77	402	296	22	22	
	25 <sup>th</sup> percentile	567	631	500	417	151	512	600	576	569	
	<b>Median</b>	602	676	647	471	340	541	730	617	618	<b>654</b>
	75 <sup>th</sup> percentile	719	721	665	525	374	593	873	618	721	
	Max	1008	808	766	579	492	873	1122	970	1122	
Scan length [cm]	Median	20	16	17	19	19	17	17	15	16	<b>19</b>
number of exams		60	36	7	2	16	7	103	123	354	

Table A.8 Paediatric patients aged 10.5 to 16 years, brain CT with CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	30	22	n	n	17	30	15	40	15	
	25 <sup>th</sup> percentile	30	41	n	n	17	30	28	40	29	
	<b>Median</b>	31	45	n	n	18	30	41	40	40	<b>40</b>
	75 <sup>th</sup> percentile	31	50	n	n	20	30	49	40	48	
	Max	31	58	n	n	21	30	52	41	58	
DLP [mGy.cm]	Min	536	58	n	n	270	471	306	576	58	
	25 <sup>th</sup> percentile	544	570	n	n	341	475	557	586	517	
	<b>Median</b>	551	699	n	n	508	479	737	617	617	<b>678</b>
	75 <sup>th</sup> percentile	559	721	n	n	1049	484	844	617	730	
	Max	566	808	n	n	2396	488	989	618	989	
Scan length [cm]	Median	18	16	n	n	19	16	17	15	16	<b>18</b>
number of exams		2	14	0	0	4	2	10	6	38	

**B: The median value for CTDI<sub>vol</sub>, DLP and scan length of all eight centres for CT of the facial bone with and without primary CM application separated by age group.**

Table B.1 Paediatric patients aged <1.5 years, facial bone CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	7	6	n	n	13	3	n	3	3	
	25 <sup>th</sup> percentile	7	6	n	n	13	4	n	3	5	
	<b>Median</b>	7	7	n	n	13	6	n	6	7	<b>7</b>
	75 <sup>th</sup> percentile	7	9	n	n	13	8	n	8	8	
	Max	7	11	n	n	13	8	n	8	13	
DLP [mGy.cm]	Min	139	71	n	n	200	31	n	41	31	
	25 <sup>th</sup> percentile	139	79	n	n	200	36	n	55	52	
	<b>Median</b>	139	87	n	n	200	41	n	75	87	<b>139</b>
	75 <sup>th</sup> percentile	139	95	n	n	200	56	n	108	121	
	Max	139	102	n	n	200	92	n	159	200	
Scan length [cm]	Median	19	19	n	n	16	10	n	15	12	<b>19</b>
number of exams		1	3	0	0	1	4	0	4	13	

Table B.2 Paediatric patients aged <1.5 years, facial bone CT with CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	11	n	n	2	n	3	n	8	2	
	25 <sup>th</sup> percentile	11	n	n	2	n	3	n	8	3	
	<b>Median</b>	11	n	n	2	n	3	n	8	6	<b>9</b>
	75 <sup>th</sup> percentile	11	n	n	2	n	3	n	8	9	
	Max	11	n	n	2	n	3	n	8	11	
DLP [mGy.cm]	Min	122	n	n	19	n	39	n	99	19	
	25 <sup>th</sup> percentile	122	n	n	19	n	39	n	99	34	
	<b>Median</b>	122	n	n	19	n	39	n	99	69	<b>105</b>
	75 <sup>th</sup> percentile	122	n	n	19	n	39	n	99	105	
	Max	122	n	n	19	n	39	n	99	122	
Scan length [cm]	Median	11	n	n	10	n	12	n	12	11	<b>12</b>
number of exams		1	0	0	1	0	1	0	1	4	

Table B.3 Paediatric patients aged 1.5 to 5.5 years, facial bone CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	1	5	n	2	5	4	4	6	1	
	25 <sup>th</sup> percentile	7	6	n	2	5	4	4	6	4	
	<b>Median</b>	16	9	n	2	5	4	5	6	6	<b>7</b>
	75 <sup>th</sup> percentile	16	12	n	2	5	4	10	8	11	
	Max	18	13	n	2	5	4	36	11	36	
DLP [mGy.cm]	Min	15	78	n	16	85	34	38	86	15	
	25 <sup>th</sup> percentile	95	81	n	17	85	34	45	90	71	
	<b>Median</b>	176	119	n	18	85	34	69	106	86	<b>113</b>
	75 <sup>th</sup> percentile	210	162	n	19	85	34	150	108	164	
	Max	258	176	n	20	85	34	809	138	809	
Scan length [cm]	Median	13	14	n	9	16	9	15	14	14	<b>15</b>
number of exams		7	4	0	2	1	1	7	9	31	

Table B.4 Paediatric patients aged 1.5 to 5.5 years, facial bone CT with CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	14	n	n	n	5	n	n	n	5	
	25 <sup>th</sup> percentile	14	n	n	n	5	n	n	n	9	
	<b>Median</b>	14	n	n	n	5	n	n	n	14	<b>12</b>
	75 <sup>th</sup> percentile	14	n	n	n	5	n	n	n	22	
	Max	14	n	n	n	5	n	n	n	29	
DLP [mGy.cm]	Min	205	n	n	n	68	n	n	n	68	
	25 <sup>th</sup> percentile	205	n	n	n	68	n	n	n	136	
	<b>Median</b>	205	n	n	n	68	n	n	n	205	<b>171</b>
	75 <sup>th</sup> percentile	205	n	n	n	68	n	n	n	471	
	Max	205	n	n	n	68	n	n	n	736	
Scan length [cm]	Median	15	n	n	n	14	n	n	n	15	<b>15</b>
number of exams		1	0	0	0	1	0	0	0	2	



Table B.5 Paediatric patients aged 5.5 to 10.5 years, facial bone CT without CM application.

		Center:	A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min		1	11	1	2	n	4	4	6	1	
	25 <sup>th</sup> percentile		11	17	2	2	n	4	4	8	4	
	<b>Median</b>		15	23	2	2	n	4	5	8	8	<b>11</b>
	75 <sup>th</sup> percentile		17	28	2	2	n	5	15	8	14	
	Max		27	34	2	2	n	12	48	16	48	
DLP [mGy.cm]	Min		13	134	22	32	n	48	36	75	13	
	25 <sup>th</sup> percentile		118	273	25	32	n	56	51	109	58	
	<b>Median</b>		172	412	29	32	n	60	62	138	123	<b>155</b>
	75 <sup>th</sup> percentile		230	551	32	32	n	66	184	155	163	
	Max		274	690	35	32	n	96	983	300	983	
Scan length [cm]	Median		11	16	16	14	n	14	12	16	14	<b>16</b>
number of exams			12	2	2	1	0	8	15	17	57	

Table B.6 Paediatric patients aged 5.5 to 10.5 years, facial bone CT with CM application.

		Center:	A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min		13	n	n	n	n	3	n	10	3	
	25 <sup>th</sup> percentile		13	n	n	n	n	4	n	10	5	
	<b>Median</b>		13	n	n	n	n	4	n	10	10	<b>12</b>
	75 <sup>th</sup> percentile		13	n	n	n	n	4	n	10	13	
	Max		13	n	n	n	n	5	n	10	16	
DLP [mGy.cm]	Min		170	n	n	n	n	65	n	182	65	
	25 <sup>th</sup> percentile		170	n	n	n	n	70	n	182	86	
	<b>Median</b>		170	n	n	n	n	76	n	182	170	<b>176</b>
	75 <sup>th</sup> percentile		170	n	n	n	n	81	n	182	182	
	Max		170	n	n	n	n	86	n	182	247	
Scan length [cm]	Median		13	n	n	n	n	20	n	18	15	<b>19</b>
number of exams			1	1	0	0	0	2	0	1	5	

Table B.7 Paediatric patients aged 10.5 to 16 years, facial bone CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	1	6	2	2	n	4	4	6	1	
	25 <sup>th</sup> percentile	1	11	2	2	n	5	7	8	5	
	<b>Median</b>	14	11	2	2	n	5	27	8	8	<b>13</b>
	75 <sup>th</sup> percentile	19	14	2	2	n	5	28	8	12	
	Max	28	15	2	2	n	12	38	16	38	
DLP [mGy.cm]	Min	18	75	30	24	n	56	56	77	18	
	25 <sup>th</sup> percentile	21	153	35	24	n	66	135	117	76	
	<b>Median</b>	155	195	40	24	n	74	268	128	129	<b>175</b>
	75 <sup>th</sup> percentile	225	216	40	24	n	81	452	138	209	
	Max	329	302	41	24	n	309	763	270	763	
Scan length [cm]	Median	13	17	17	12	n	15	16	16	15	<b>17</b>
number of exams		14	9	3	1	0	16	25	37	105	

Table B.8 Paediatric patients aged 10.5 to 16 years, facial bone CT with CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	17	n	5	n	n	n	n	40	5	
	25 <sup>th</sup> percentile	17	n	5	n	n	n	n	40	16	
	<b>Median</b>	17	n	5	n	n	n	n	40	18	<b>28</b>
	75 <sup>th</sup> percentile	17	n	5	n	n	n	n	40	19	
	Max	17	n	5	n	n	n	n	40	40	
DLP [mGy.cm]	Min	197	n	70	n	n	n	n	617	79	
	25 <sup>th</sup> percentile	197	n	70	n	n	n	n	617	262	
	<b>Median</b>	197	n	70	n	n	n	n	617	332	<b>407</b>
	75 <sup>th</sup> percentile	197	n	70	n	n	n	n	617	404	
	Max	197	n	70	n	n	n	n	617	810	
Scan length [cm]	Median	12	n	15	n	n	n	n	16	18	<b>15</b>
number of exams		1	0	1	0	0	0	0	1	3	

**C: The median value for CTDI<sub>vol</sub>, DLP and scan length of all eight centres for CT of the petrous bone with and without primary CM application separated by age group.**

Table C.1 Paediatric patients aged <1.5 years, petrous bone CT without CM application

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	17	26	n	n	13	17	n	11	11	
	25 <sup>th</sup> percentile	17	28	n	n	13	18	n	11	13	
	<b>Median</b>	17	29	n	n	13	19	n	11	17	<b>19</b>
	75 <sup>th</sup> percentile	17	31	n	n	13	20	n	11	26	
	Max	17	32	n	n	13	21	n	13	35	
DLP [mGy.cm]	Min	105	163	n	n	70	76	n	62	62	
	25 <sup>th</sup> percentile	105	170	n	n	70	86	n	84	85	
	<b>Median</b>	105	177	n	n	70	95	n	85	114	<b>105</b>
	75 <sup>th</sup> percentile	114	184	n	n	70	105	n	102	179	
	Max	122	191	n	n	70	114	n	179	240	
Scan length [cm]	Median	6	6	n	n	5	5	n	8	6	<b>6</b>
number of exams		3	2	0	0	1	2	0	5	13	

Paediatric patients aged <1.5 years, petrous bone CT with CM application:

No such examinations were recorded at any of the participating centres.

Table C.2 Paediatric patients aged 1.5 to 5.5 years, petrous bone CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	17	27	1	44	17	14	n	3	1	
	25 <sup>th</sup> percentile	17	35	1	44	17	18	n	11	11	
	<b>Median</b>	17	36	1	44	17	21	n	11	18	<b>29</b>
	75 <sup>th</sup> percentile	19	40	1	44	17	23	n	11	35	
	Max	21	54	1	44	17	24	n	16	54	
DLP [mGy.cm]	Min	118	162	12	186	88	98	n	43	12	
	25 <sup>th</sup> percentile	133	218	12	269	88	104	n	67	88	
	<b>Median</b>	147	260	12	352	88	110	n	79	114	<b>204</b>
	75 <sup>th</sup> percentile	165	265	12	393	88	142	n	89	222	
	Max	182	378	12	435	88	228	n	106	435	
Scan length [cm]	Median	7	7	9	8	5	7	n	7	7	<b>7</b>
number of exams		3	6	1	3	1	7	0	11	32	

Paediatric patients aged 1.5 to 5.5 years, petrous bone CT with CM application:

No such examinations were recorded at any of the participating centres.

Table C.3 Paediatric patients aged 5.5 to 10.5 years, petrous bone CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	17	43	1	44	16	16	n	15	1	
	25 <sup>th</sup> percentile	21	43	1	44	17	18	n	15	15	
	Median	21	43	1	44	17	22	n	15	18	<b>32</b>
	75 <sup>th</sup> percentile	21	43	1	44	17	23	n	15	40	
	Max	21	43	1	44	18	26	n	16	54	
DLP [mGy.cm]	Min	131	291	10	261	74	106	n	93	10	
	25 <sup>th</sup> percentile	163	291	10	274	101	121	n	106	107	
	Median	171	291	10	293	102	125	n	115	131	<b>231</b>
	75 <sup>th</sup> percentile	188	291	11	300	106	141	n	124	264	
	Max	201	291	11	386	112	170	n	209	397	
Scan length [cm]	Median	8	7	7	7	6	7	n	8	7	<b>7</b>
number of exams		6	1	2	6	6	7	0	16	44	

Table C.4 Paediatric patients aged 5.5 to 10.5 years, petrous bone with CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
CTDI [mGy]	Min	21	n	n	n	n	n	n	n	21	
	25 <sup>th</sup> percentile	21	n	n	n	n	n	n	n	21	
	Median	21	n	n	n	n	n	n	n	21	<b>21</b>
	75 <sup>th</sup> percentile	21	n	n	n	n	n	n	n	21	
	Max	21	n	n	n	n	n	n	n	21	
DLP [mGy.cm]	Min	212	n	n	n	n	n	n	n	212	
	25 <sup>th</sup> percentile	212	n	n	n	n	n	n	n	212	
	Median	212	n	n	n	n	n	n	n	212	<b>212</b>
	75 <sup>th</sup> percentile	212	n	n	n	n	n	n	n	212	
	Max	212	n	n	n	n	n	n	n	212	
Scan length [cm]	Median	10	n	n	n	n	n	n	n	10	<b>10</b>
number of exams		1	0	0	0	0	0	0	0	1	

Table C.5 Paediatric patients aged 10.5 to 16 years, petrous bone CT without CM application.

Center:		A	B	C	D	E	F	H	I	All data	DRL 75
<b>CTDI [mGy]</b>	Min	21	35	n	n	20	16	n	8	8	
	25 <sup>th</sup> percentile	21	51	n	n	20	18	n	15	15	
	<b>Median</b>	21	54	n	n	20	27	n	15	21	<b>27</b>
	75 <sup>th</sup> percentile	21	54	n	n	20	27	n	15	28	
	Max	21	54	n	n	20	28	n	16	54	
<b>DLP [mGy.cm]</b>	Min	131	162	n	n	123	116	n	70	70	
	25 <sup>th</sup> percentile	185	325	n	n	123	134	n	102	131	
	<b>Median</b>	201	365	n	n	123	147	n	117	180	<b>201</b>
	75 <sup>th</sup> percentile	212	430	n	n	123	172	n	132	228	
	Max	238	450	n	n	123	196	n	184	450	
<b>Scan length [cm]</b>	Median	9	8	n	n	6	7	n	8	8	<b>8</b>
<b>number of exams</b>		11	8	0	0	1	5	0	11	36	

Paediatric patients aged 10.5 to 16 years, petrous bone with CM application:

No such examinations were recorded at any of the participating centres.